

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023054.D
 Acq On : 27 Oct 2021 13:38
 Operator : SY/MD
 Sample : VV1027WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK236

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	73304	74815	14.32%	1.847%
2	1.568	155	164	174	rBV	57052	65586	12.56%	1.619%
3	2.108	321	332	345	rBV	107155	154736	29.63%	3.821%
4	2.510	448	457	470	rVB	10928	18482	3.54%	0.456%
5	3.047	614	624	634	rBV7	4631	9469	1.81%	0.234%
6	3.905	880	891	922	rBV	38710	150246	28.77%	3.710%
7	4.352	1014	1030	1057	rBV	91206	237483	45.47%	5.864%
8	5.050	1230	1247	1271	rBV3	209444	522269	100.00%	12.895%
9	5.619	1409	1424	1452	rBV	146491	306452	58.68%	7.566%
10	5.908	1505	1514	1530	rVB6	7388	15971	3.06%	0.394%
11	6.072	1550	1565	1596	rBV	122283	257735	49.35%	6.364%
12	6.989	1840	1850	1869	rBV2	55424	106233	20.34%	2.623%
13	7.320	1940	1953	1973	rBV	241416	425088	81.39%	10.496%
14	7.397	1973	1977	1990	rVB6	4983	8468	1.62%	0.209%
15	7.625	2038	2048	2067	rBV2	32364	60053	11.50%	1.483%
16	8.095	2184	2194	2230	rBV2	190830	433556	83.01%	10.705%
17	8.853	2415	2430	2450	rBV	235996	387084	74.12%	9.557%
18	10.217	2843	2854	2870	rBV	73982	119764	22.93%	2.957%
19	11.249	3165	3175	3195	rBV	209621	326916	62.60%	8.072%
20	11.625	3281	3292	3311	rBV	220674	350085	67.03%	8.644%
21	14.043	4033	4044	4054	rBV	11807	19645	3.76%	0.485%




Sum of corrected areas: 4050136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023054.D
Acq On : 27 Oct 2021 13:38
Operator : SY/MD
Sample : VV1027WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

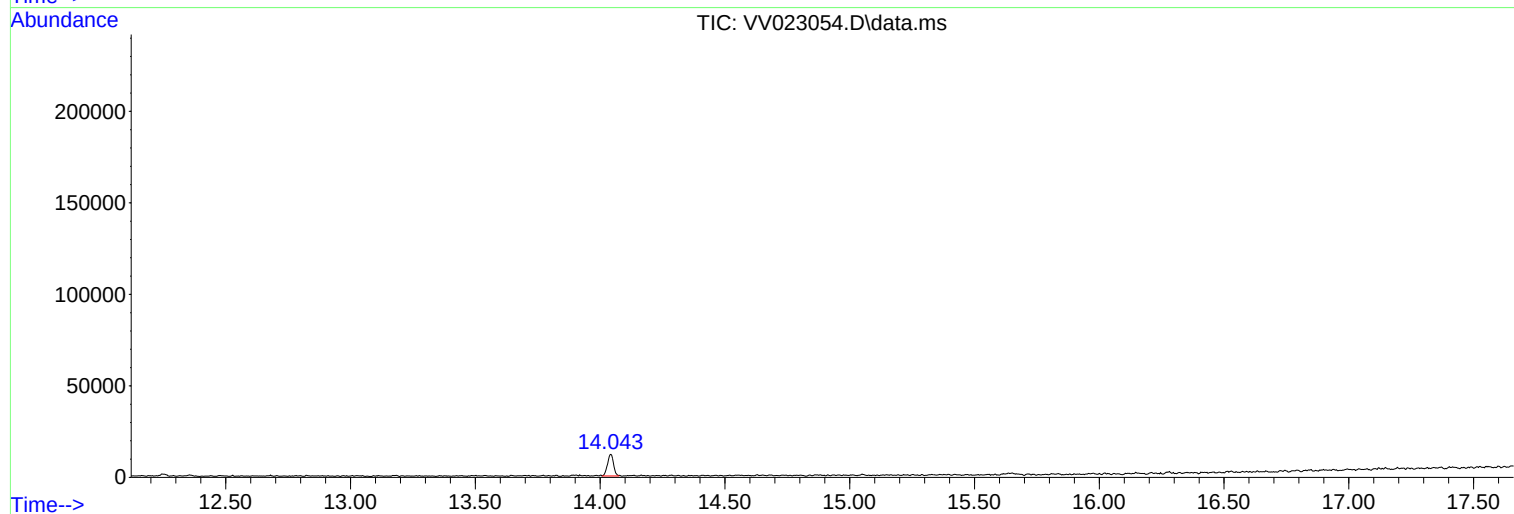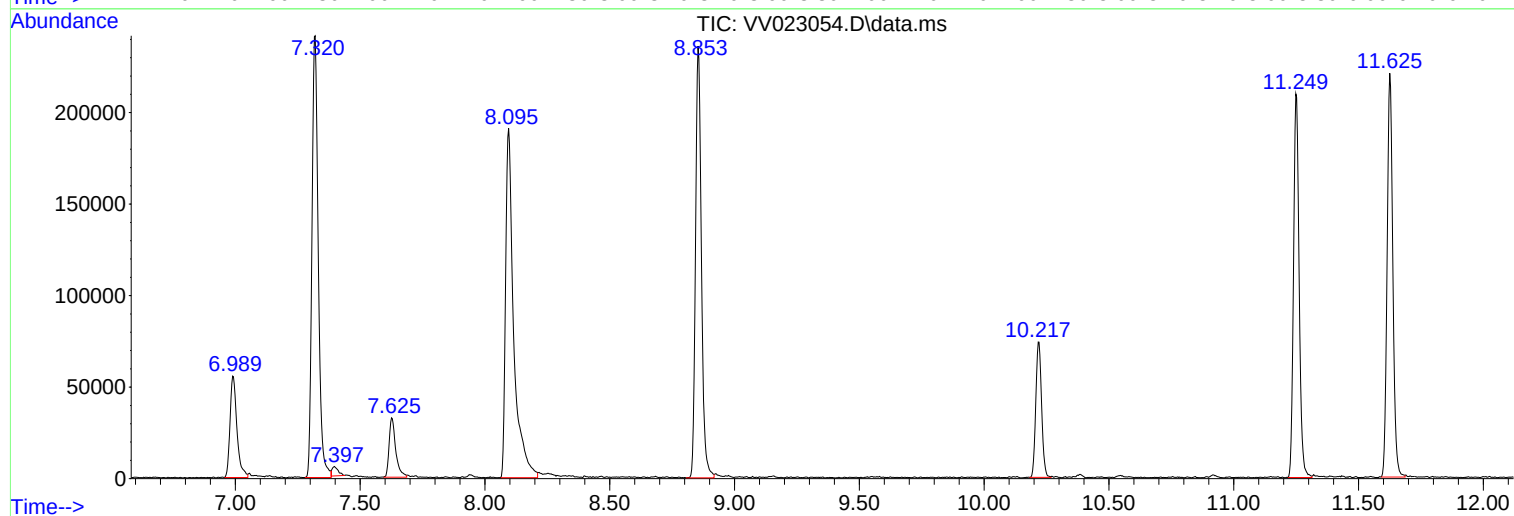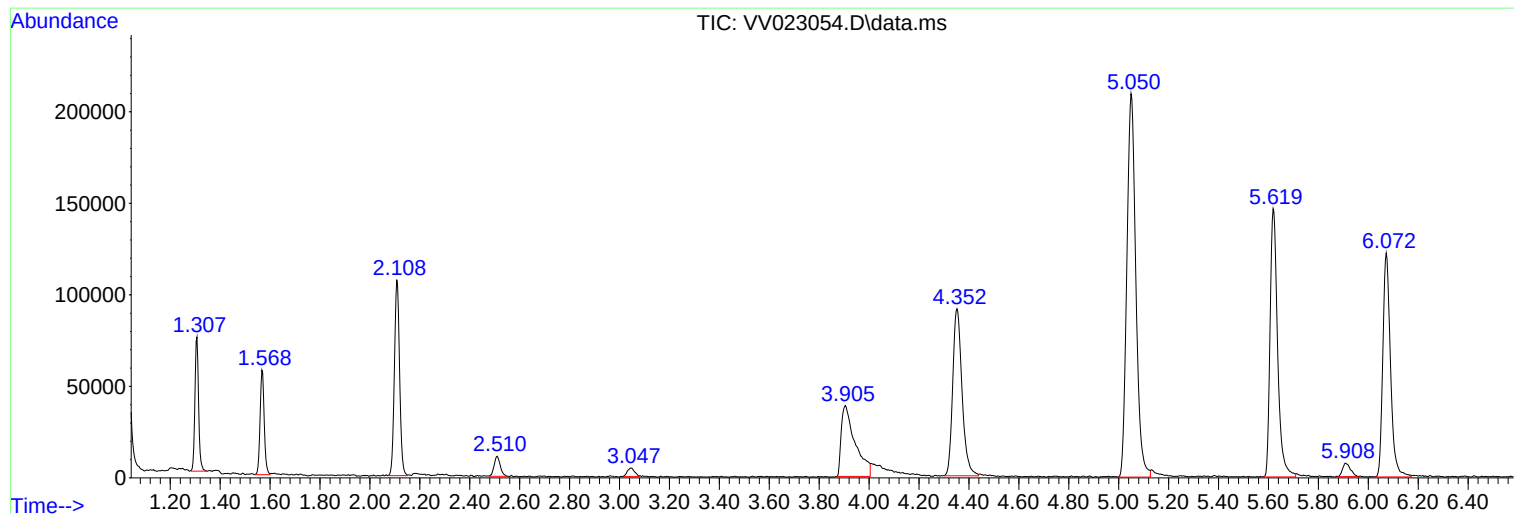

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023054.D
Acq On : 27 Oct 2021 13:38
Operator : SY/MD
Sample : VV1027WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023054.D
Acq On : 27 Oct 2021 13:38
Operator : SY/MD
Sample : VV1027WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK236

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
