

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023062.D
 Acq On : 27 Oct 2021 16:46
 Operator : SY/MD
 Sample : M4277-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGB9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	80489	83401	15.91%	2.020%
2	1.568	156	164	178	rBV	58840	68552	13.08%	1.660%
3	2.108	322	332	346	rBV	87634	127330	24.29%	3.084%
4	3.899	878	889	921	rBV	47334	177012	33.76%	4.287%
5	4.352	1012	1030	1055	rBV4	98408	287819	54.90%	6.970%
6	5.050	1231	1247	1270	rBV3	209637	524263	100.00%	12.696%
7	5.619	1412	1424	1451	rBV	149276	311743	59.46%	7.550%
8	5.915	1507	1516	1518	rBV7	4151	5504	1.05%	0.133%
9	6.072	1553	1565	1590	rBV	121780	256570	48.94%	6.214%
10	6.989	1838	1850	1872	rBV	55823	106748	20.36%	2.585%
11	7.320	1941	1953	1970	rBV	237103	422846	80.66%	10.240%
12	7.400	1970	1978	1991	rVB2	9816	21192	4.04%	0.513%
13	7.625	2038	2048	2071	rBV	31388	60221	11.49%	1.458%
14	7.982	2149	2159	2172	rVB2	11892	21396	4.08%	0.518%
15	8.091	2183	2193	2230	rBV2	217834	450676	85.96%	10.914%
16	8.853	2419	2430	2457	rBV	237068	389719	74.34%	9.438%
17	10.217	2842	2854	2866	rBV2	81841	131833	25.15%	3.193%
18	11.249	3165	3175	3197	rVB	210034	331011	63.14%	8.016%
19	11.625	3279	3292	3314	rBV	223828	351358	67.02%	8.509%




Sum of corrected areas: 4129194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023062.D
Acq On : 27 Oct 2021 16:46
Operator : SY/MD
Sample : M4277-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

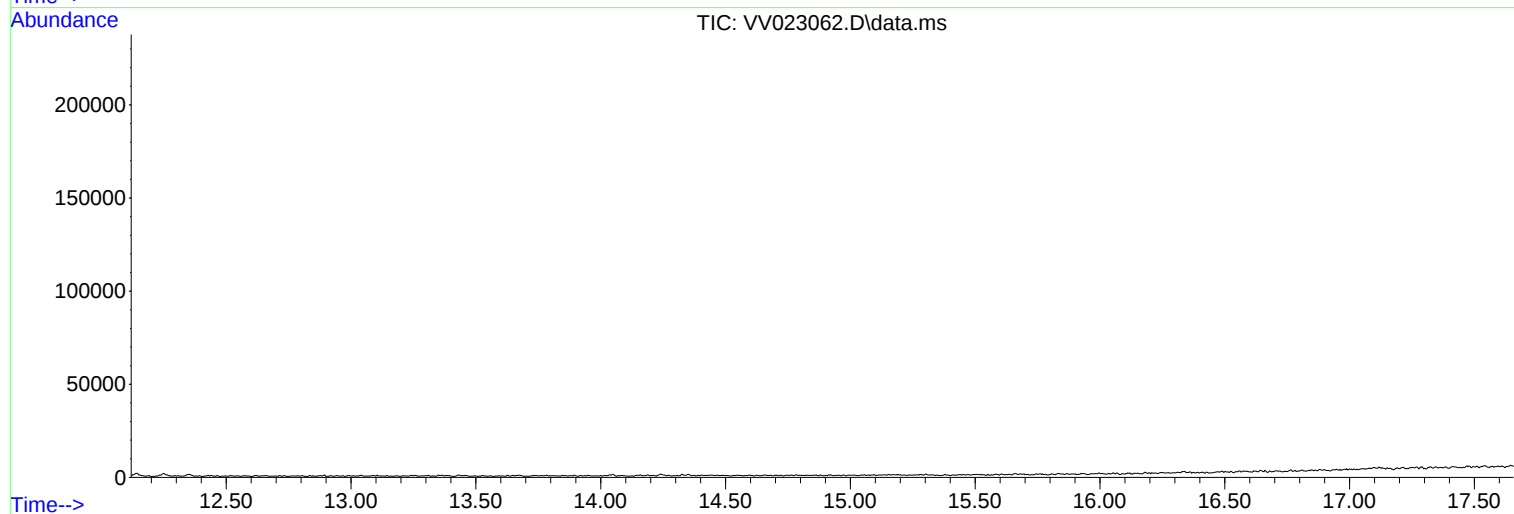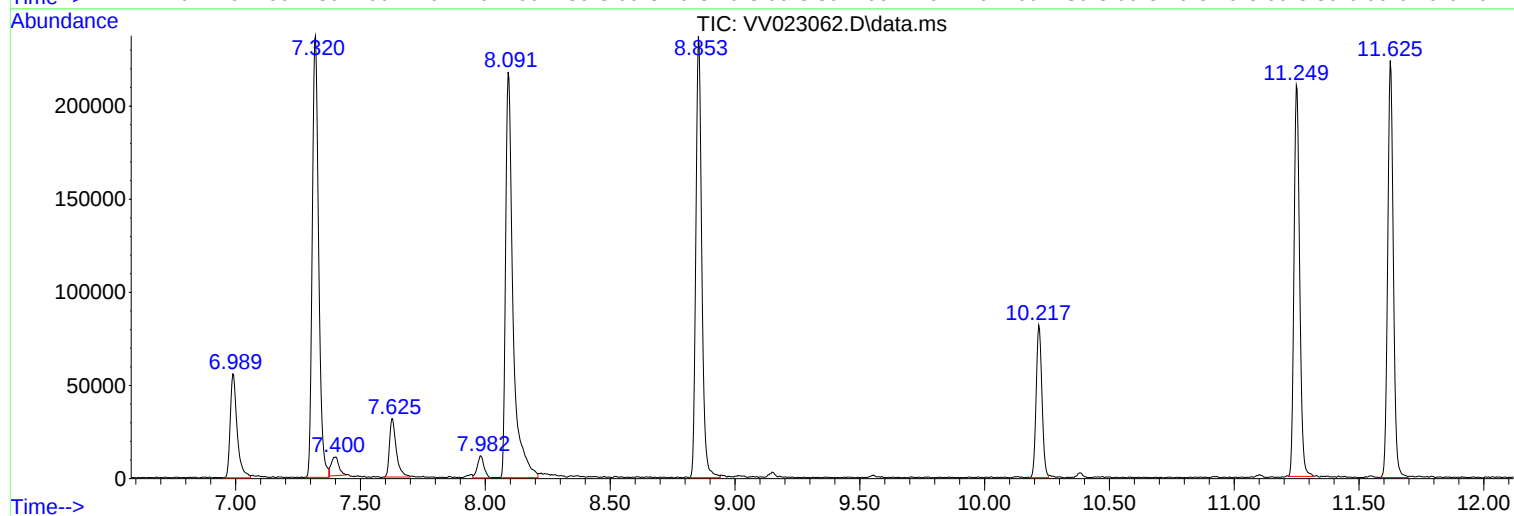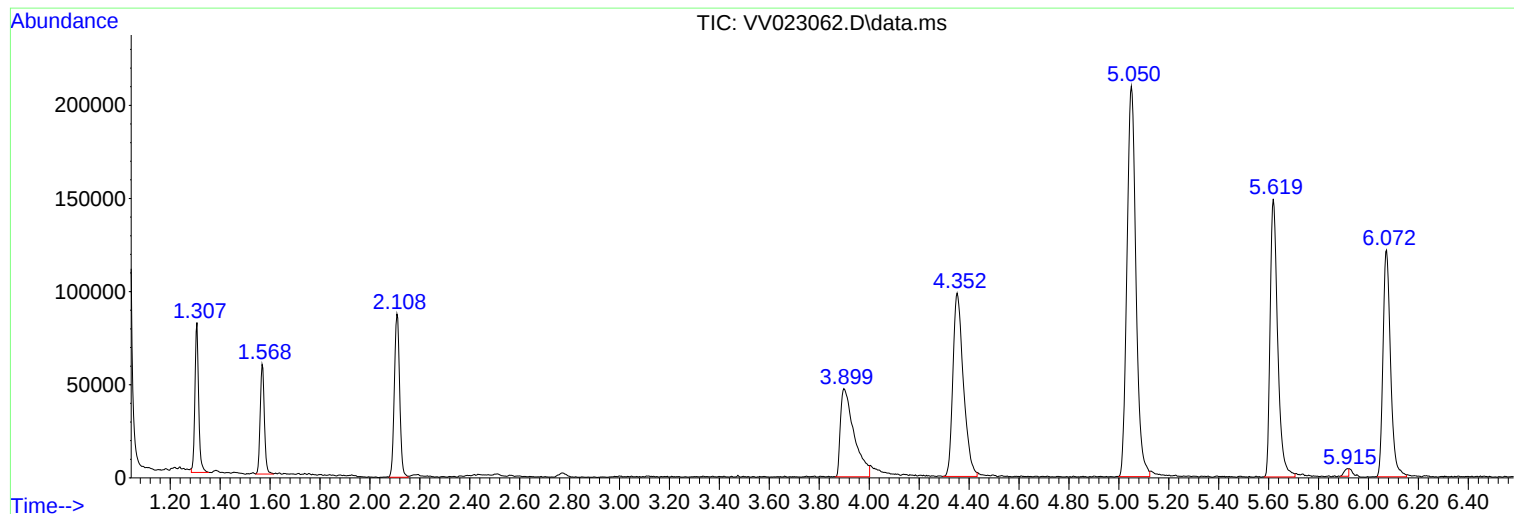

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023062.D
Acq On : 27 Oct 2021 16:46
Operator : SY/MD
Sample : M4277-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023062.D
Acq On : 27 Oct 2021 16:46
Operator : SY/MD
Sample : M4277-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
