

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023064.D
 Acq On : 27 Oct 2021 17:34
 Operator : SY/MD
 Sample : M4278-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	96	rVB	78253	81457	15.12%	1.953%
2	1.568	155	164	174	rBV	57419	66842	12.40%	1.602%
3	2.108	321	332	347	rVB	124736	167400	31.07%	4.013%
4	3.899	879	889	930	rBV	46458	187790	34.85%	4.502%
5	4.352	1010	1030	1055	rBV	93160	238936	44.34%	5.728%
6	5.050	1228	1247	1281	rBV2	213184	538852	100.00%	12.917%
7	5.619	1413	1424	1454	rBV	152483	313941	58.26%	7.526%
8	5.915	1503	1516	1527	rBV7	5492	12545	2.33%	0.301%
9	6.072	1552	1565	1592	rBV2	121009	256862	47.67%	6.157%
10	6.989	1839	1850	1866	rBV	54531	106484	19.76%	2.553%
11	7.317	1941	1952	1972	rBV	241858	429363	79.68%	10.292%
12	7.400	1975	1978	1991	rVB6	4925	7492	1.39%	0.180%
13	7.625	2036	2048	2066	rBV2	33382	63103	11.71%	1.513%
14	8.092	2183	2193	2230	rBV2	217390	460800	85.52%	11.046%
15	8.854	2418	2430	2449	rBV	243279	392067	72.76%	9.398%
16	10.217	2842	2854	2870	rBV	80808	130825	24.28%	3.136%
17	10.384	2897	2906	2915	rVB3	3835	5826	1.08%	0.140%
18	11.252	3165	3176	3194	rBV	210051	335845	62.33%	8.051%
19	11.625	3280	3292	3310	rBV	220629	354933	65.87%	8.508%
20	14.043	4030	4044	4058	rVB	12682	20286	3.76%	0.486%


Sum of corrected areas: 4171649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023064.D
Acq On : 27 Oct 2021 17:34
Operator : SY/MD
Sample : M4278-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

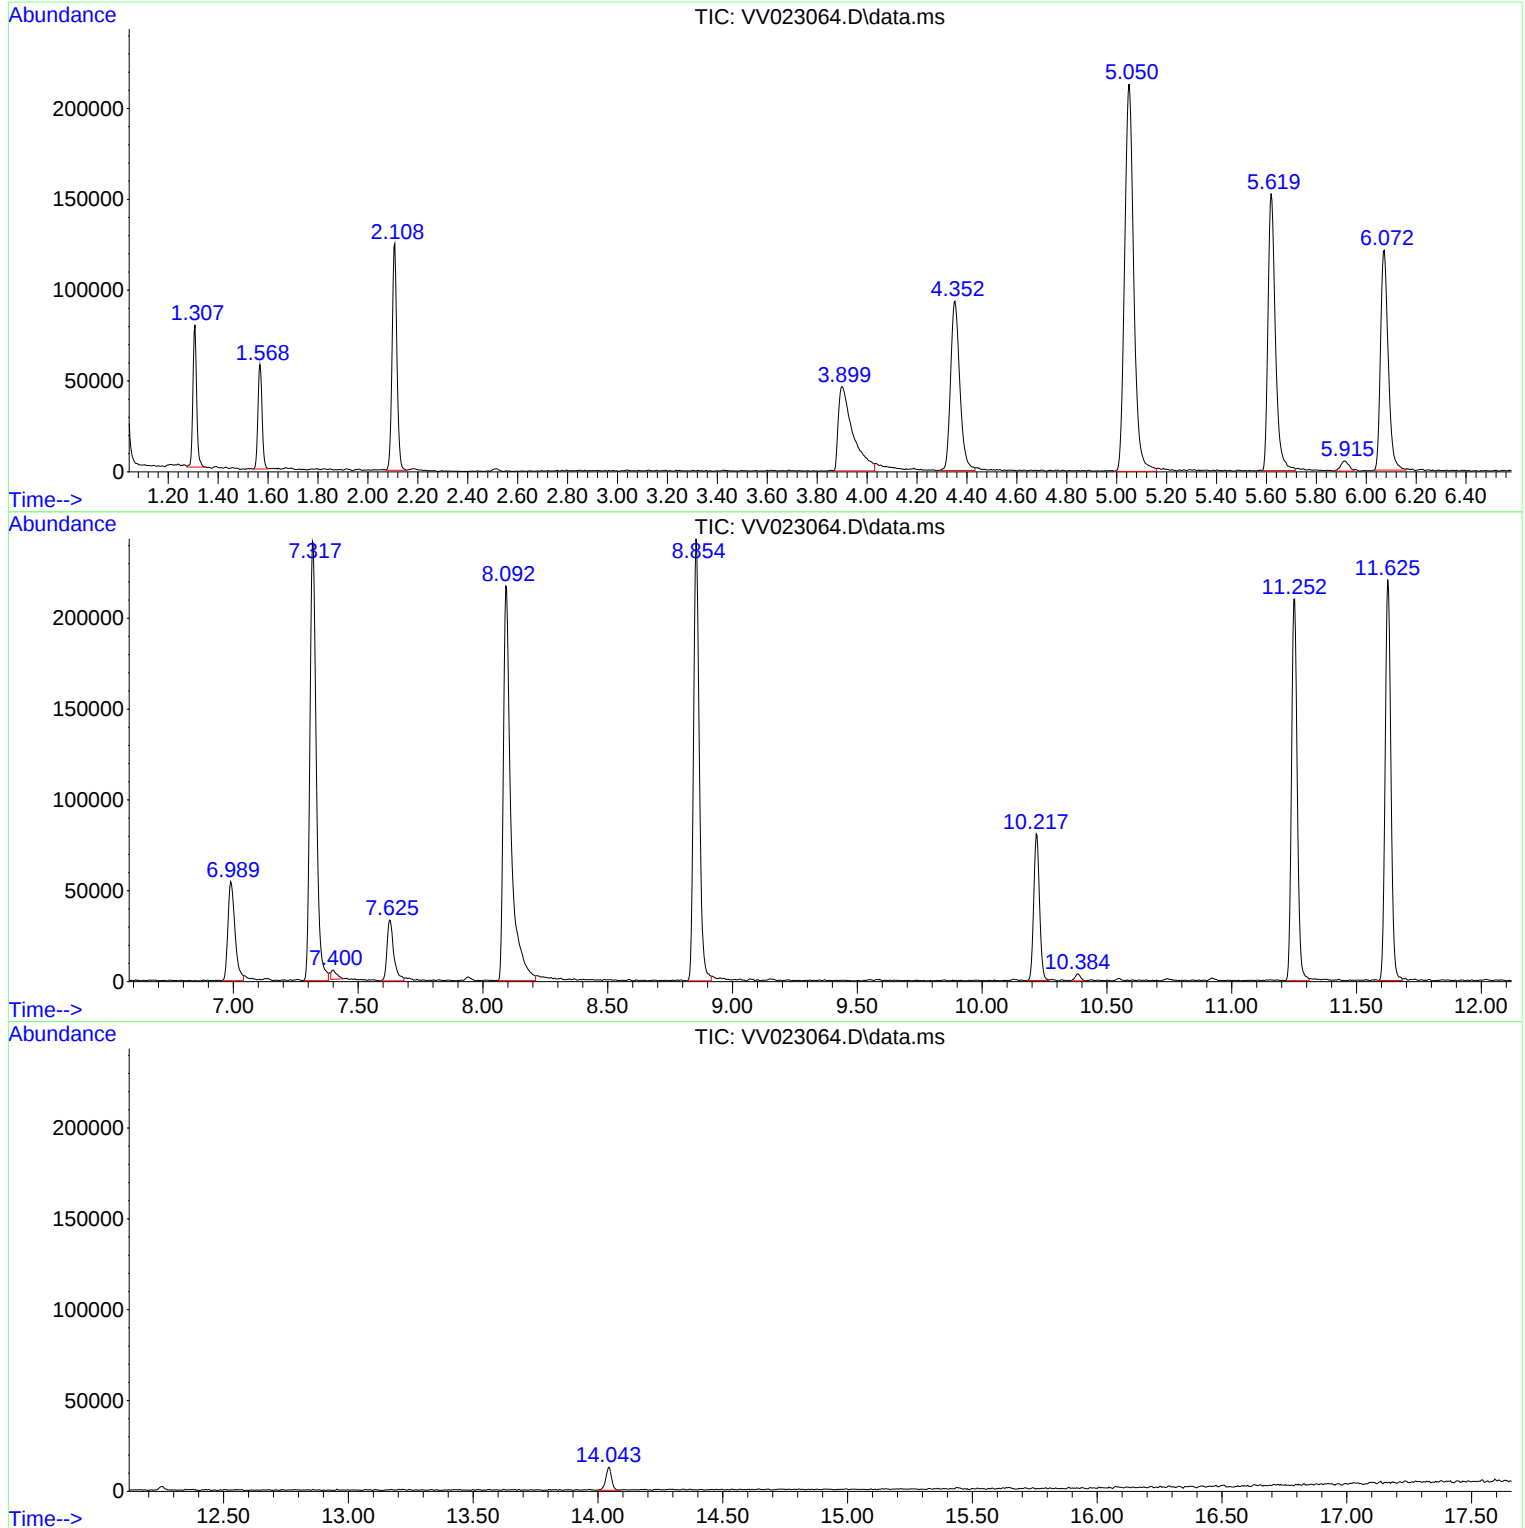

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023064.D
Acq On : 27 Oct 2021 17:34
Operator : SY/MD
Sample : M4278-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023064.D
Acq On : 27 Oct 2021 17:34
Operator : SY/MD
Sample : M4278-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc