

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023065.D
 Acq On : 27 Oct 2021 18:22
 Operator : SY/MD
 Sample : M4364-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG320

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	79817	86274	16.82%	2.000%
2	1.568	155	164	174	rBV	53316	59839	11.67%	1.387%
3	1.947	275	282	290	rBV4	4860	6310	1.23%	0.146%
4	2.108	322	332	347	rVB	120635	176247	34.36%	4.086%
5	3.192	656	669	687	rBV	26808	57196	11.15%	1.326%
6	3.909	874	892	928	rBV3	117107	401888	78.35%	9.317%
7	4.349	1014	1029	1053	rBV	89145	226998	44.25%	5.262%
8	4.613	1096	1111	1121	rBV4	9400	23084	4.50%	0.535%
9	5.050	1231	1247	1271	rBV2	204377	512967	100.00%	11.892%
10	5.619	1412	1424	1449	rBV	149199	306107	59.67%	7.096%
11	5.918	1503	1517	1529	rBV7	15122	34731	6.77%	0.805%
12	6.072	1551	1565	1591	rBV	117833	248246	48.39%	5.755%
13	6.989	1839	1850	1868	rBV2	49295	94312	18.39%	2.186%
14	7.317	1941	1952	1972	rBV	230991	413457	80.60%	9.585%
15	7.625	2036	2048	2065	rBV2	29698	55174	10.76%	1.279%
16	8.092	2180	2193	2226	rBV	216230	431135	84.05%	9.995%
17	8.854	2419	2430	2450	rBV	234531	384293	74.92%	8.909%
18	10.217	2841	2854	2867	rBV	80548	129845	25.31%	3.010%
19	11.249	3162	3175	3191	rBV	206349	325722	63.50%	7.551%
20	11.625	3281	3292	3310	rBV	212423	339775	66.24%	7.877%




Sum of corrected areas: 4313600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023065.D
Acq On : 27 Oct 2021 18:22
Operator : SY/MD
Sample : M4364-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

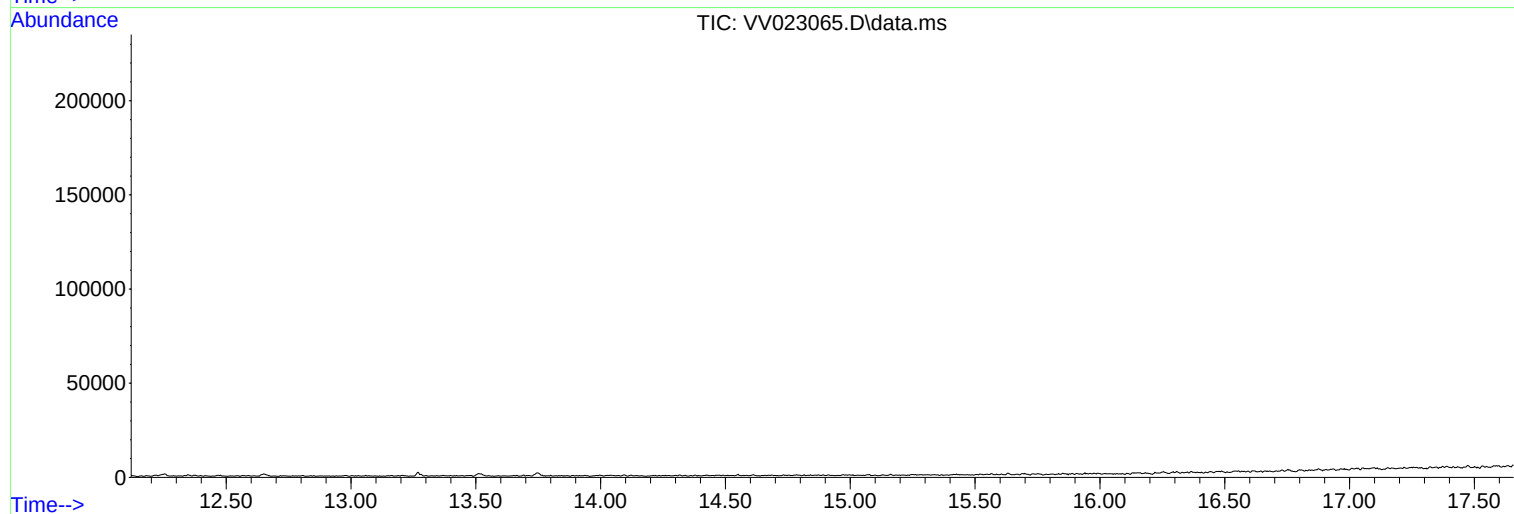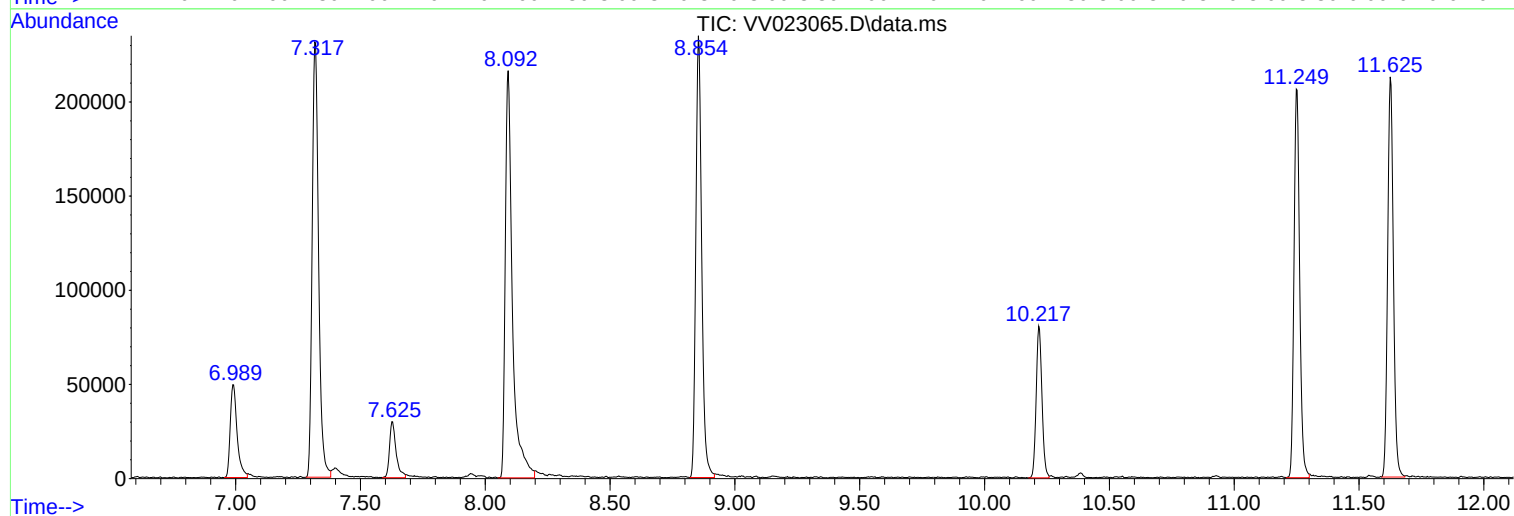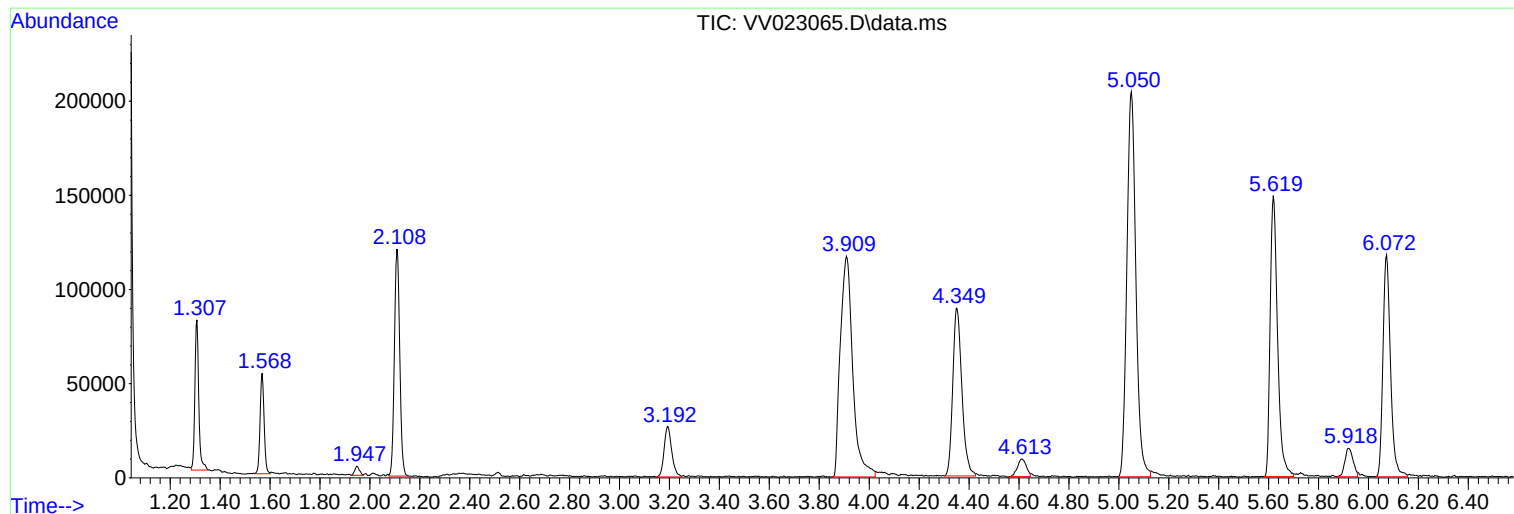

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023065.D
Acq On : 27 Oct 2021 18:22
Operator : SY/MD
Sample : M4364-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023065.D
Acq On : 27 Oct 2021 18:22
Operator : SY/MD
Sample : M4364-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG320

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
