

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032755.D
 Acq On : 28 Oct 2023 20:34
 Operator : SY/MD
 Sample : 05103-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 30 01:57:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	126888	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	146653	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	62988	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	47249	4.534	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.600%	
7) Chloroethane-d5	1.532	69	47673	5.383	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	107.600%	
11) 1,1-Dichloroethene-d2	2.060	65	19438	4.156	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	83.200%	
20) 2-Butanone-d5	3.802	46	92709	41.197	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	82.400%	
24) Chloroform-d	4.253	84	86262	4.985	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	4.947	65	45007	5.268	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.400%	
32) Benzene-d6	4.963	84	173284	4.963	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
36) 1,2-Dichloropropane-d6	5.992	67	53964	5.337	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.800%	
41) Toluene-d8	7.246	98	155661	4.398	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.000%	
43) trans-1,3-Dichloroprop...	7.561	79	19422	4.353	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.000%	
46) 2-Hexanone-d5	8.031	63	75992	42.979	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	85.960%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	42521	4.729	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152	61286	5.959	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	119.200%	
Target Compounds					Qvalue	
13) Acetone	2.127	43	3451	1.553	ug/L	72
42) Toluene	7.330	91	5378	0.100	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032755.D
Acq On : 28 Oct 2023 20:34
Operator : SY/MD
Sample : 05103-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 30 01:57:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

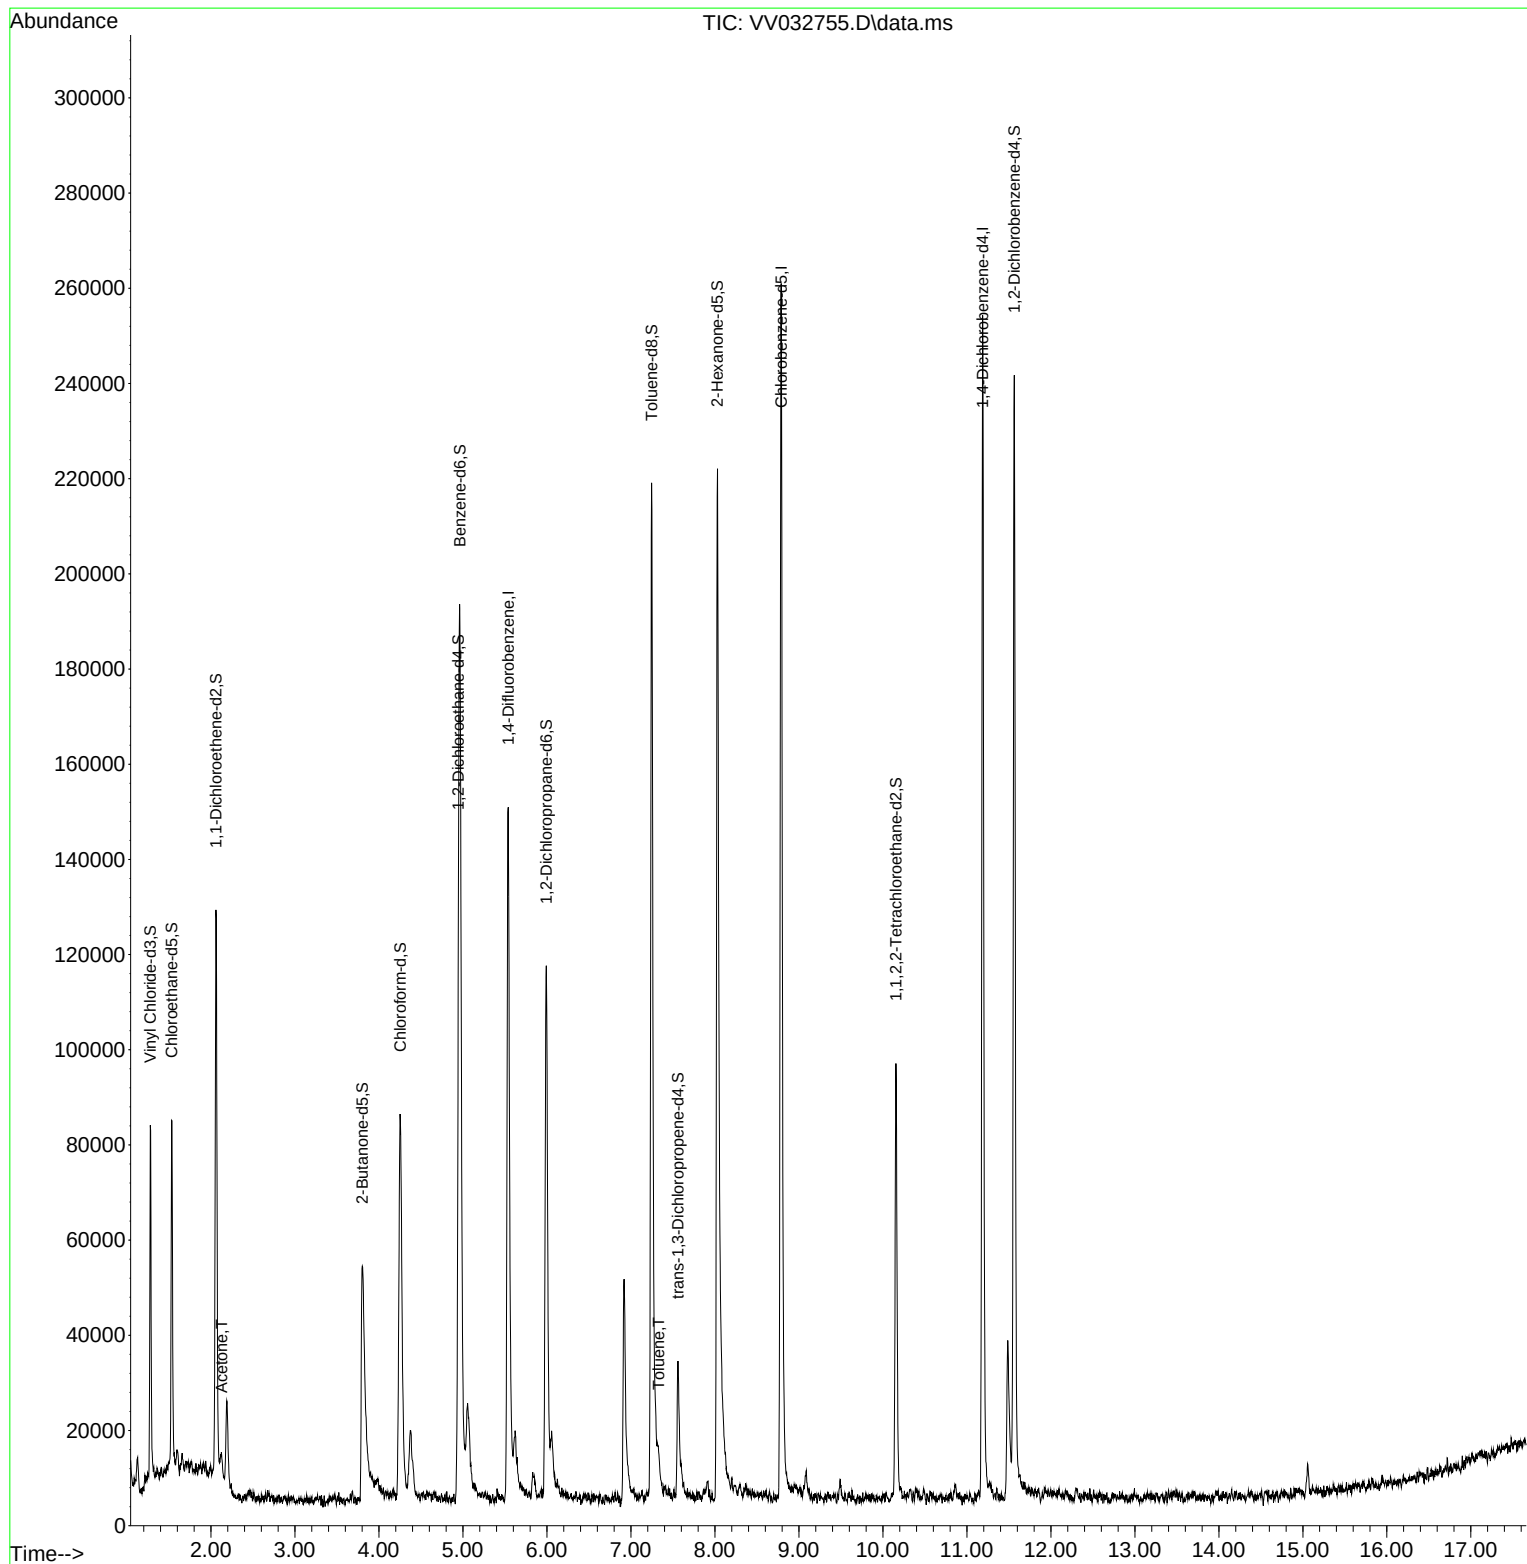

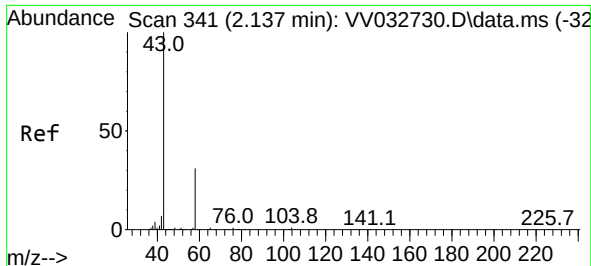

#13

Acetone

Concen: 1.553 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV032755.D

Acq: 28 Oct 2023 20:34

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 3451

Ion Ratio Lower Upper

43 100

58 39.4 0.0 50.6

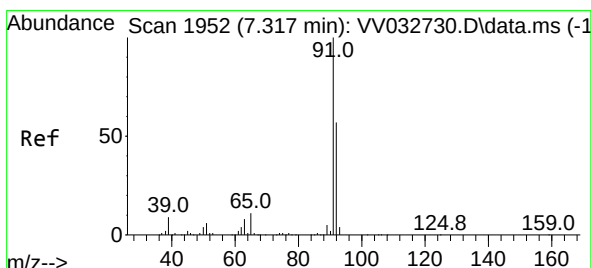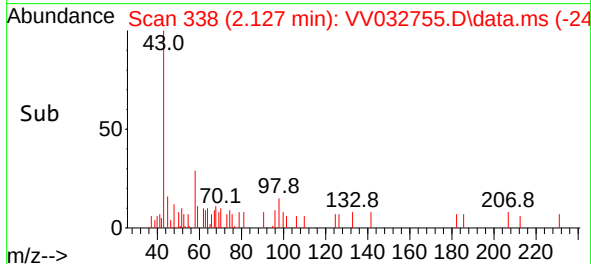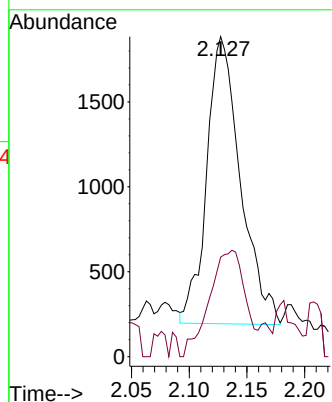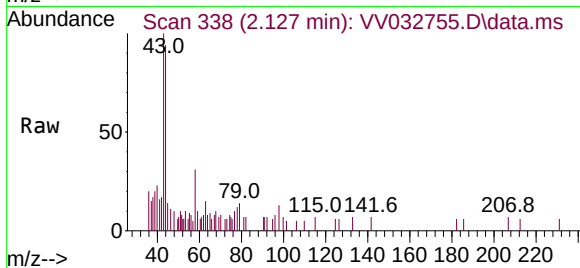

#42

Toluene

Concen: 0.100 ug/L

RT: 7.330 min Scan# 1956

Delta R.T. 0.013 min

Lab File: VV032755.D

Acq: 28 Oct 2023 20:34

Tgt Ion: 91 Resp: 5378

Ion Ratio Lower Upper

91 100

92 51.2 39.9 74.1

