




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032736.D
 Acq On : 28 Oct 2023 12:53
 Operator : SY/MD
 Sample : 04993-09DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 30 01:52:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 10/31/2023

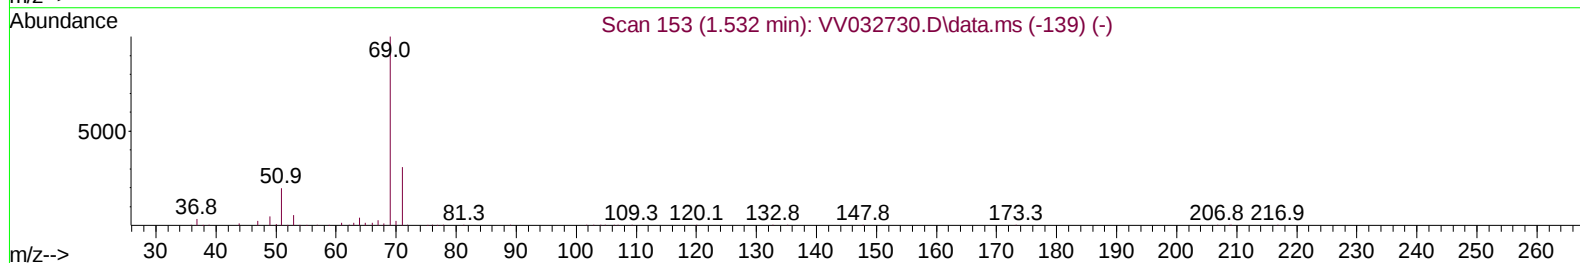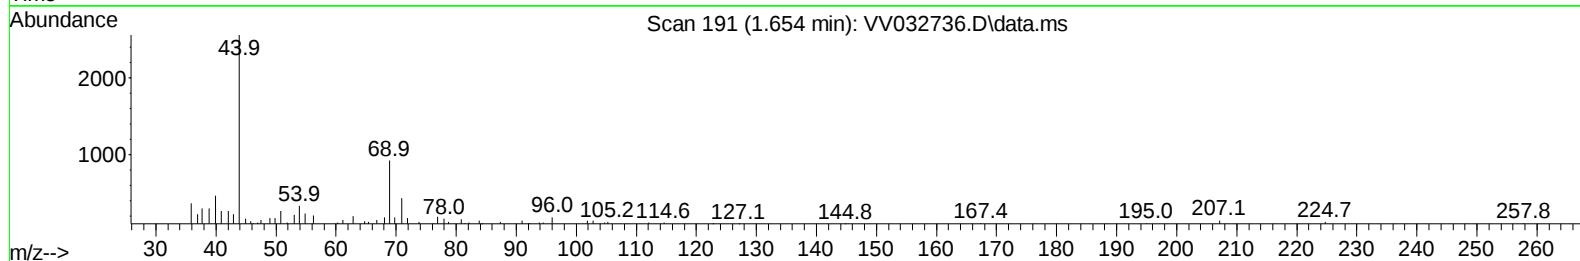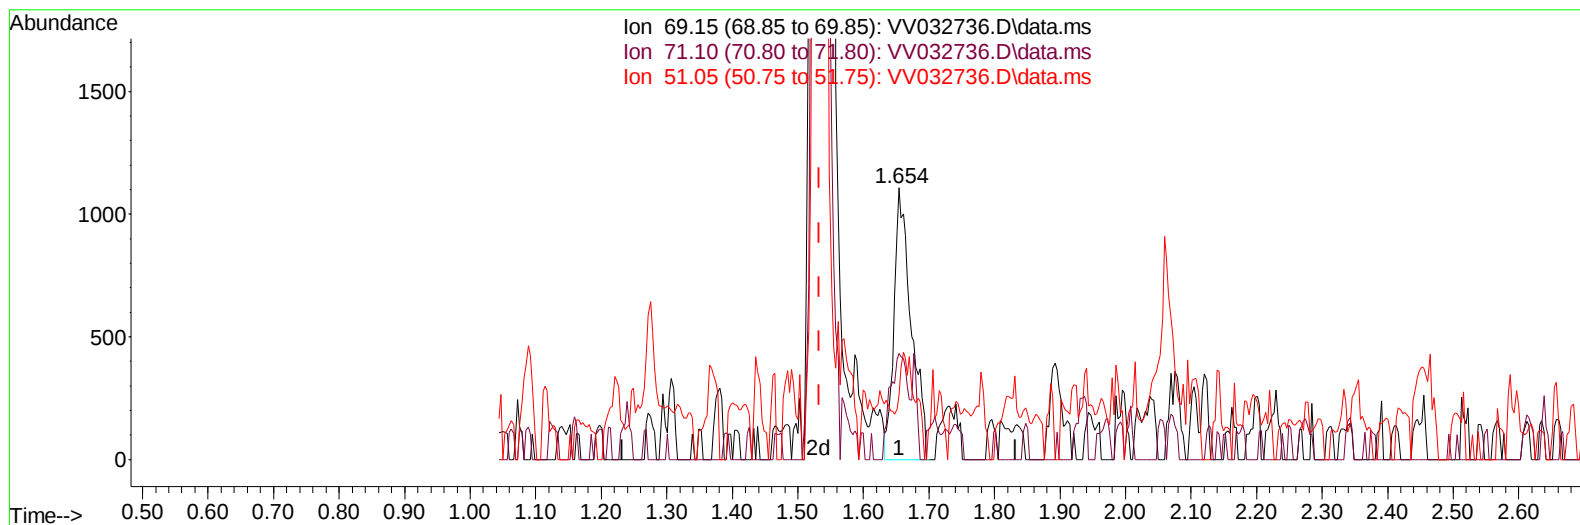

TIC: VV032736.D\data.ms

(7) Chloroethane-d5 (S)

1.654min (+ 0.122) 0.21 ug/L

response	2011	
Ion	Exp%	Act%
69.15	100.00	100.00
71.10	33.20	41.27
51.05	28.90	37.05
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032736.D
 Acq On : 28 Oct 2023 12:53
 Operator : SY/MD
 Sample : 04993-09DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 30 01:52:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 10/31/2023

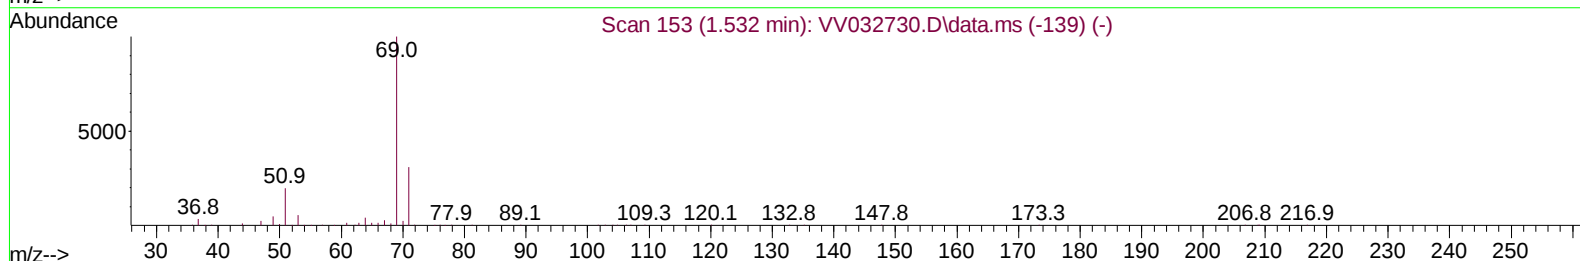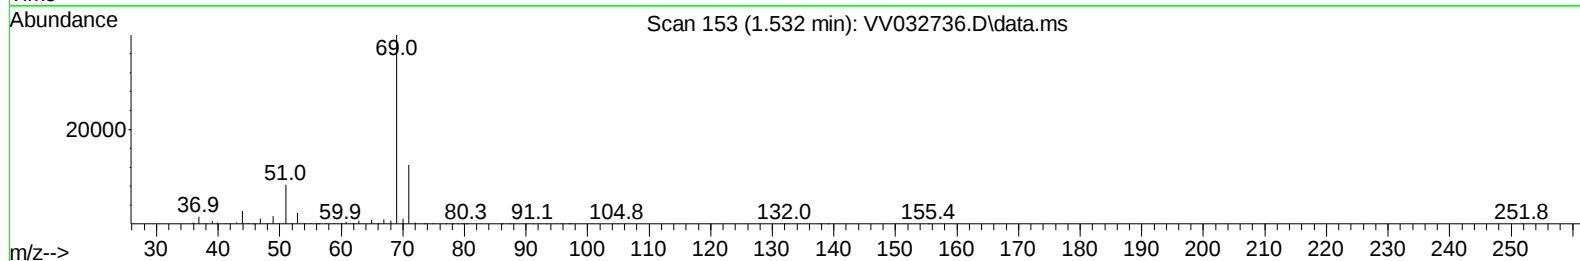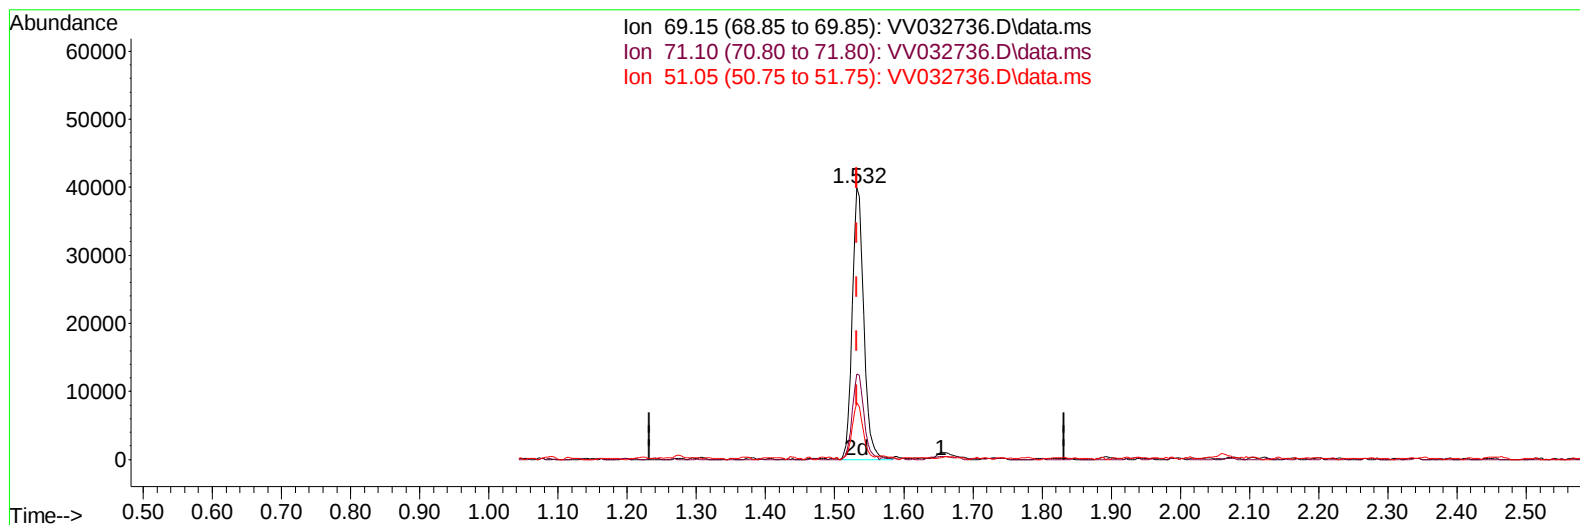

TIC: VV032736.D\data.ms

(7) Chloroethane-d5 (S)

1.532min (-0.000) 4.71 ug/L m

response 45991

Ion	Exp%	Act%
69.15	100.00	100.00
71.10	33.20	1.80#
51.05	28.90	1.62#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032736.D
 Acq On : 28 Oct 2023 12:53
 Operator : SY/MD
 Sample : 04993-09DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 30 01:52:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 10/31/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.538	114		139918	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117		159832	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		68178	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		50257	4.374	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%	
7) Chloroethane-d5	1.532	69		45991m	4.710	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.200%	
11) 1,1-Dichloroethene-d2	2.060	65		21302	4.130	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.600%	
20) 2-Butanone-d5	3.818	46		98985	39.890	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.780%	
24) Chloroform-d	4.252	84		92599	4.853	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%	
26) 1,2-Dichloroethane-d4	4.947	65		47781	5.072	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%	
32) Benzene-d6	4.963	84		180342	4.739	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	5.992	67		55498	5.036	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%	
41) Toluene-d8	7.246	98		164470	4.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.561	79		21249	4.370	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.400%	
46) 2-Hexanone-d5	8.030	63		83876	43.526	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.060%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		46392	4.734	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152		60357	5.422	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.400%	
Target Compounds							
47) Tetrachloroethene	7.905	164		195859	16.467	ug/L	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032736.D
Acq On : 28 Oct 2023 12:53
Operator : SY/MD
Sample : 04993-09DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3DL

Manual IntegrationsAPPROVED

Quant Time: Oct 30 01:52:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
Supervised By :Mahesh Dadoda 10/31/2023

