

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032699.D
 Acq On : 27 Oct 2023 21:22
 Operator : SY/MD
 Sample : 05055-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F8

Quant Time: Oct 28 00:28:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 28 00:17:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	134206	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	151031	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	66872	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	51151	4.641	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.800%
7) Chloroethane-d5	1.532	69	48131	5.139	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.800%
11) 1,1-Dichloroethene-d2	2.060	65	20741	4.192	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.800%
20) 2-Butanone-d5	3.802	46	92202	38.738	ug/L	-0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.480%
24) Chloroform-d	4.252	84	89620	4.897	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
26) 1,2-Dichloroethane-d4	4.947	65	46837	5.183	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	4.963	84	180341	5.015	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
36) 1,2-Dichloropropane-d6	5.992	67	55070	5.289	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.800%
41) Toluene-d8	7.246	98	159438	4.374	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	7.561	79	20153	4.386	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.800%
46) 2-Hexanone-d5	8.030	63	77253	42.425	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.860%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	43852	4.736	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	11.564	152	58635	5.370	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.400%
Target Compounds						Qvalue
3) Chloromethane	1.217	50	3482	0.214	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032699.D
Acq On : 27 Oct 2023 21:22
Operator : SY/MD
Sample : 05055-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F8

Quant Time: Oct 28 00:28:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 28 00:17:24 2023
Response via : Initial Calibration

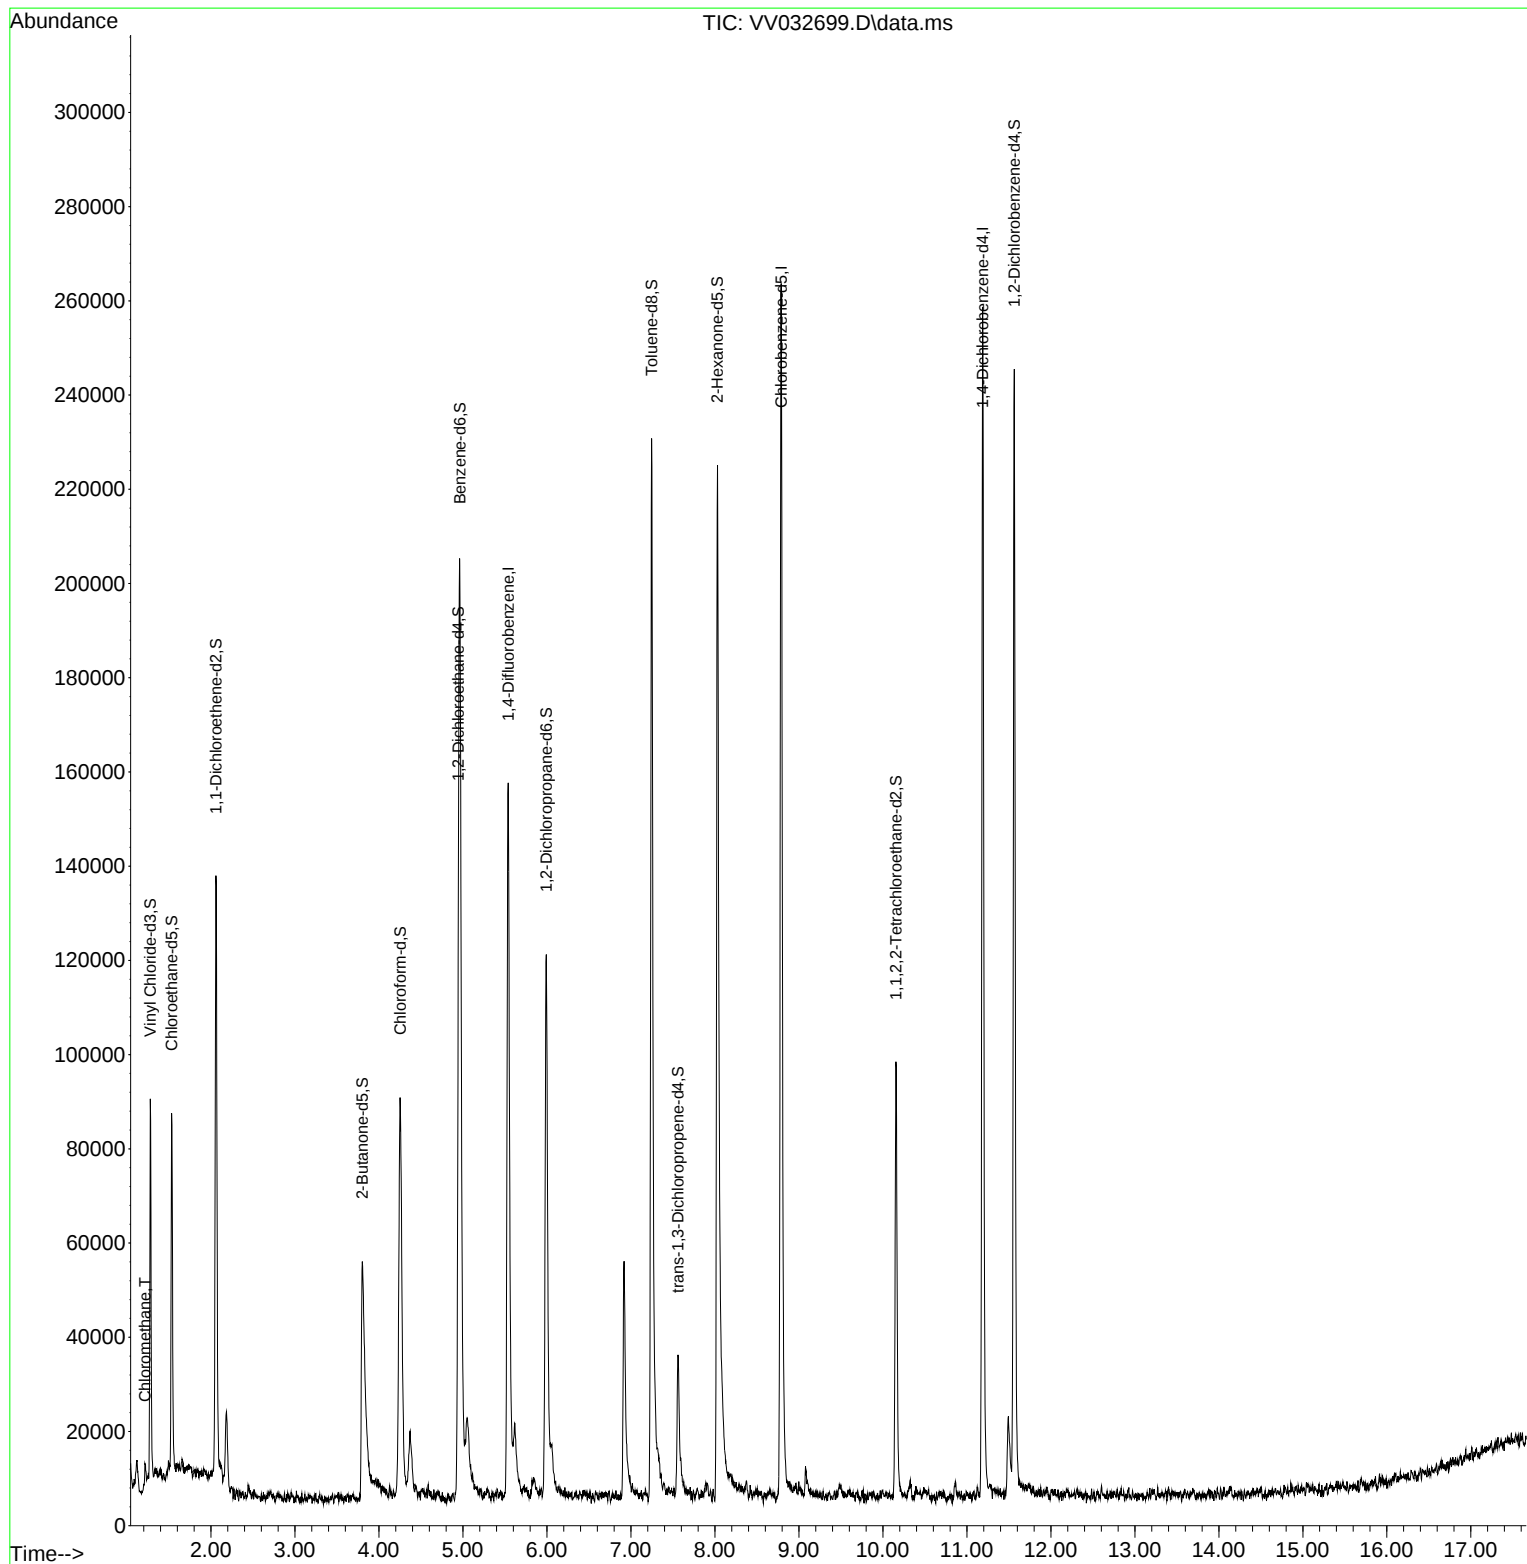

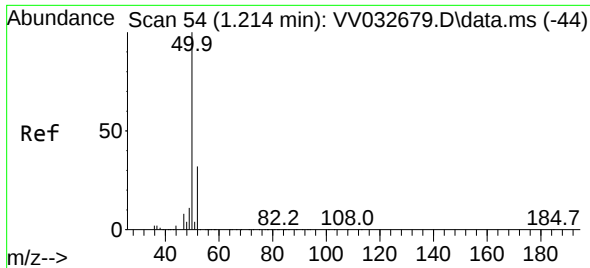

#3
 Chloromethane
 Concen: 0.214 ug/L
 RT: 1.217 min Scan# 51
 Delta R.T. 0.003 min
 Lab File: VV032699.D
 Acq: 27 Oct 2023 21:22

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F8

Tgt Ion: 50 Resp: 3482
 Ion Ratio Lower Upper
 50 100
 52 40.6 22.3 41.5

