

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032721.D
 Acq On : 28 Oct 2023 06:41
 Operator : SY/MD
 Sample : 05019-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49A2

Quant Time: Oct 30 01:13:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 28 02:08:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	133235	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	157009	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	67697	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	50398	4.606	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.200%
7) Chloroethane-d5	1.532	69	45174	4.858	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.059	65	20900	4.255	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.200%
20) 2-Butanone-d5	3.809	46	97996	41.472	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.940%
24) Chloroform-d	4.252	84	88513	4.872	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	4.947	65	44920	5.008	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.200%
32) Benzene-d6	4.963	84	178852	4.784	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	5.992	67	53208	4.915	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.246	98	158589	4.185	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.800%
43) trans-1,3-Dichloroprop...	7.561	79	19764	4.138	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.800%
46) 2-Hexanone-d5	8.030	63	76403	40.361	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.720%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	43201	4.488	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	11.564	152	59565	5.388	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						Qvalue
3) Chloromethane	1.217	50	11854	0.735	ug/L	93
13) Acetone	2.137	43	9241	3.961	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032721.D
Acq On : 28 Oct 2023 06:41
Operator : SY/MD
Sample : 05019-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49A2

Quant Time: Oct 30 01:13:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 28 02:08:41 2023
Response via : Initial Calibration




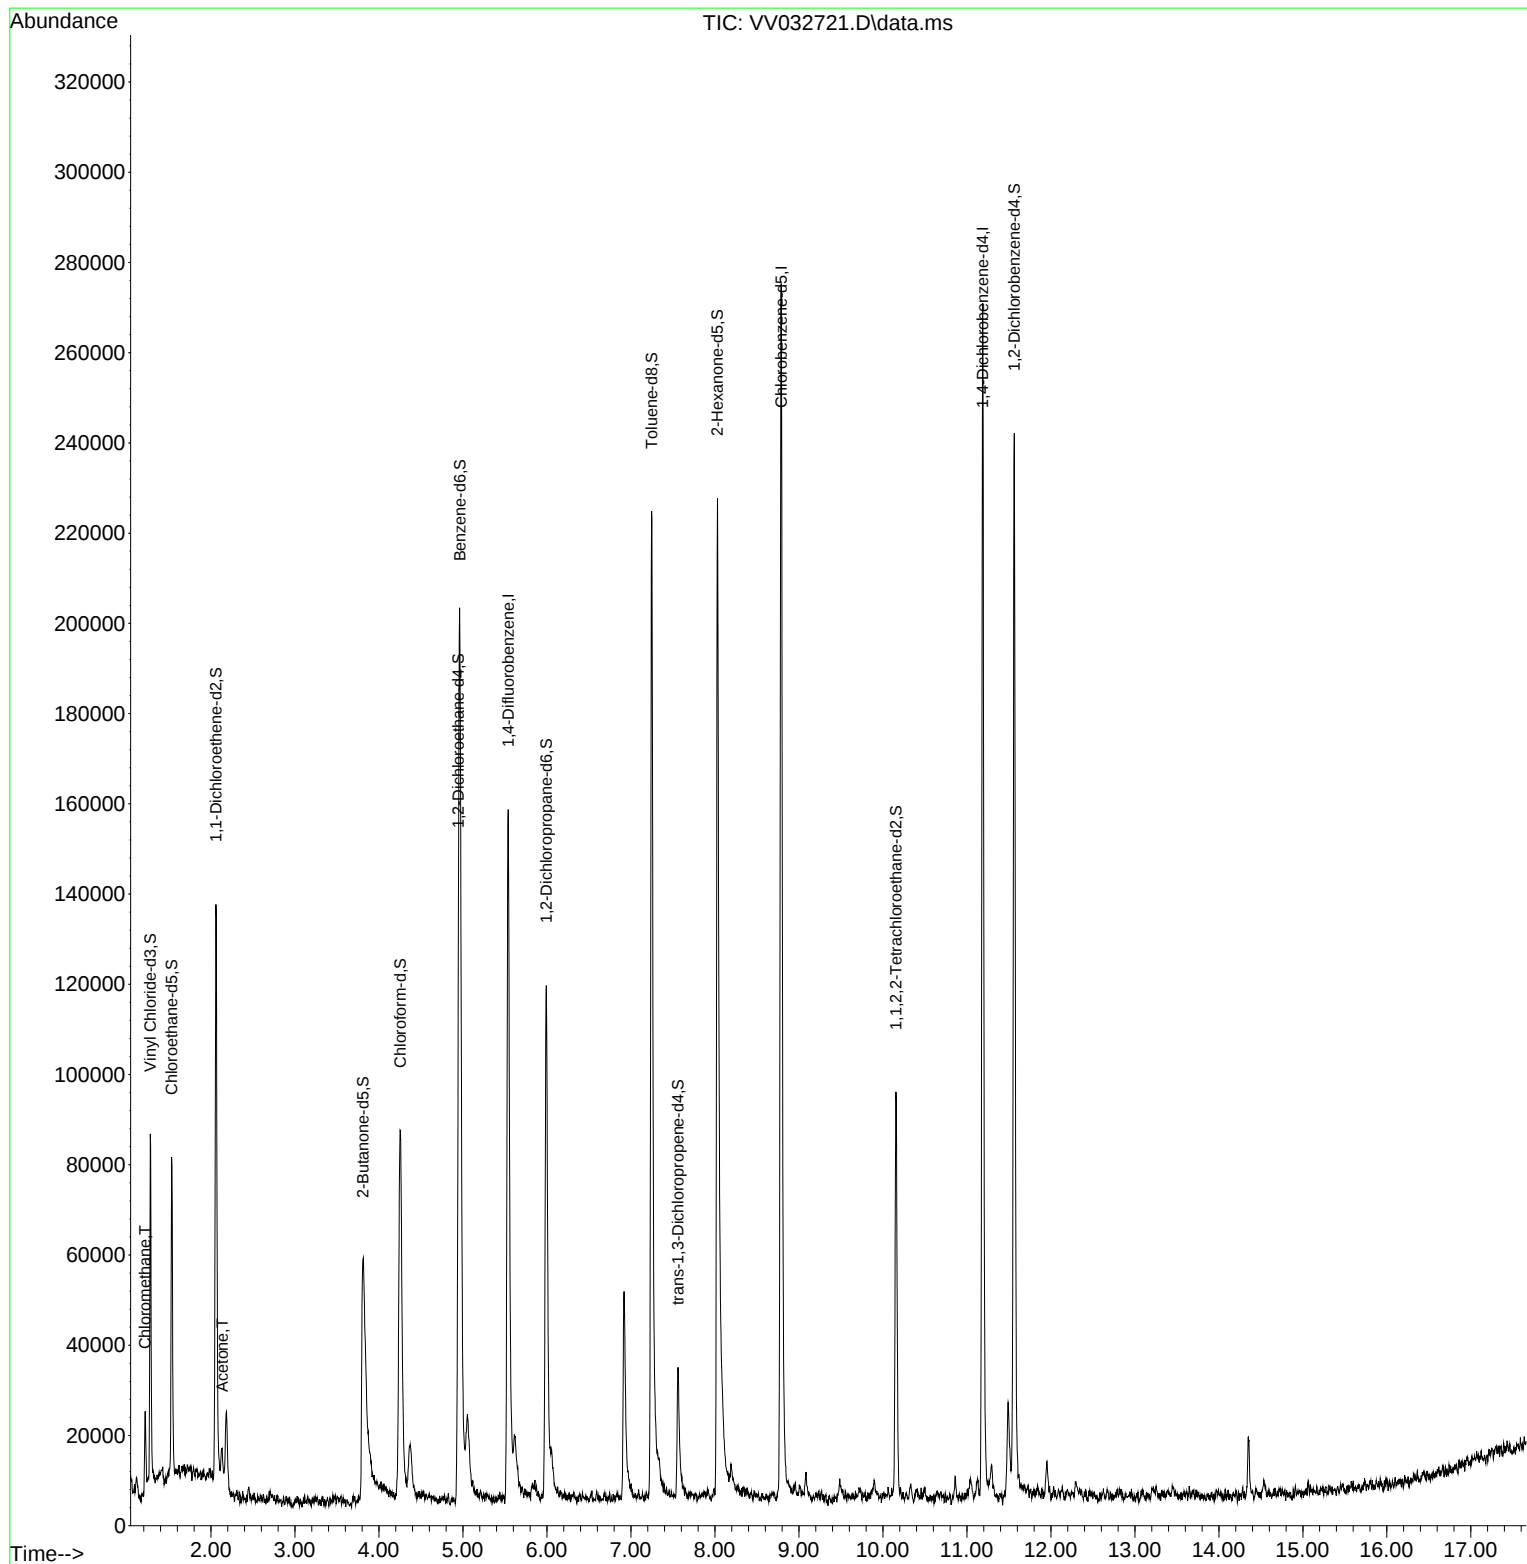


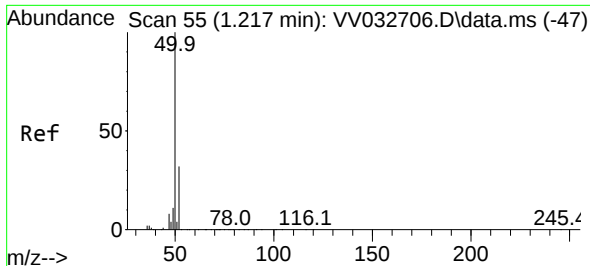

#3
Chloromethane
Concen: 0.735 ug/L
RT: 1.217 min Scan# 51
Delta R.T. 0.000 min
Lab File: VV032721.D
Acq: 28 Oct 2023 06:41

Instrument :
MSVOA_V
ClientSampleId :
A49A2

Tgt Ion: 50 Resp: 11854
Ion Ratio Lower Upper
50 100
52 35.6 22.3 41.5

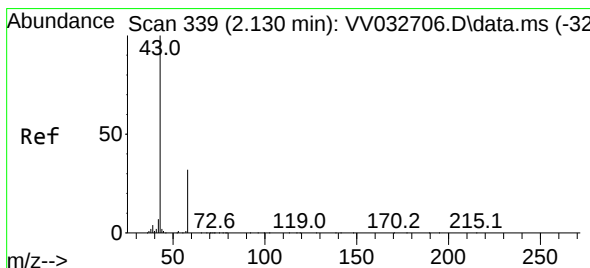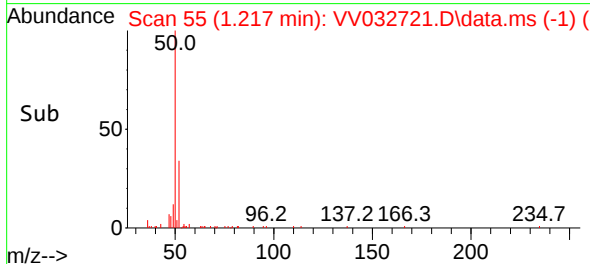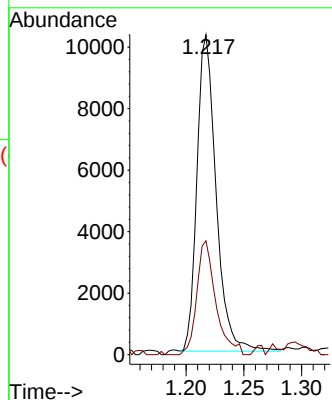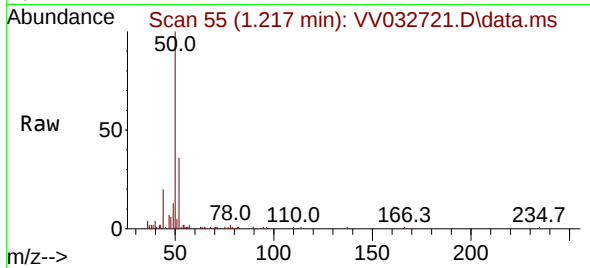

#13
Acetone
Concen: 3.961 ug/L
RT: 2.137 min Scan# 341
Delta R.T. 0.006 min
Lab File: VV032721.D
Acq: 28 Oct 2023 06:41

Tgt Ion: 43 Resp: 9241
Ion Ratio Lower Upper
43 100
58 23.2 0.0 50.6

