

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032743.D
 Acq On : 28 Oct 2023 15:41
 Operator : SY/MD
 Sample : 05019-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49H7

Quant Time: Oct 30 01:54:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	128932	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	148210	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	65335	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	47019	4.440	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.800%
7) Chloroethane-d5	1.532	69	47827	5.315	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.200%
11) 1,1-Dichloroethene-d2	2.060	65	19795	4.165	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.200%
20) 2-Butanone-d5	3.802	46	94393	41.280	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.560%
24) Chloroform-d	4.252	84	85928	4.887	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	4.947	65	44762	5.156	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	4.963	84	173728	4.923	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
36) 1,2-Dichloropropane-d6	5.992	67	53833	5.268	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.400%
41) Toluene-d8	7.246	98	155938	4.360	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.561	79	19766	4.384	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.600%
46) 2-Hexanone-d5	8.030	63	74128	41.484	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.960%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	43740	4.814	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	57968	5.434	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.600%
Target Compounds						Qvalue
13) Acetone	2.130	43	3971	1.759	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032743.D
Acq On : 28 Oct 2023 15:41
Operator : SY/MD
Sample : 05019-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H7

Quant Time: Oct 30 01:54:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

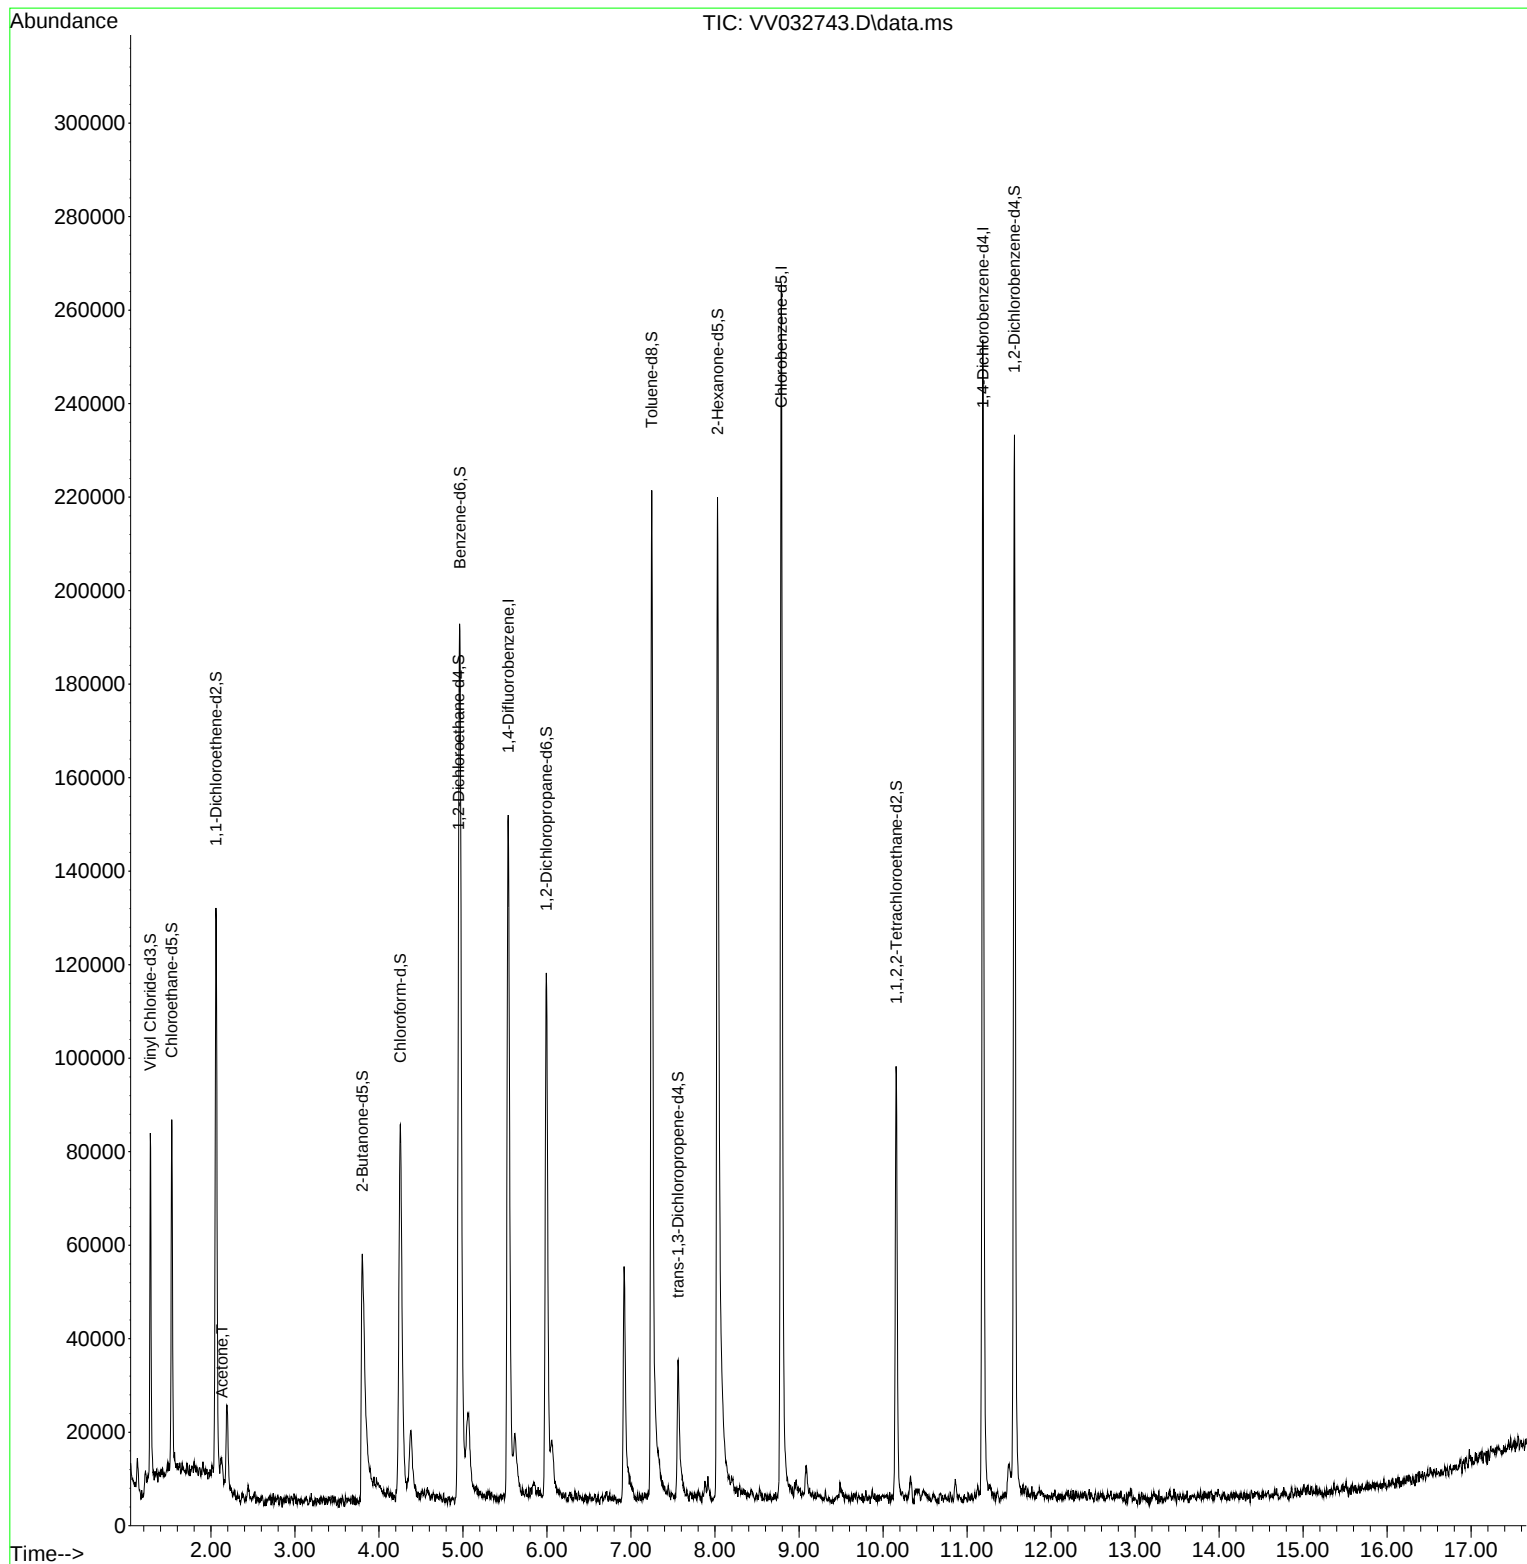

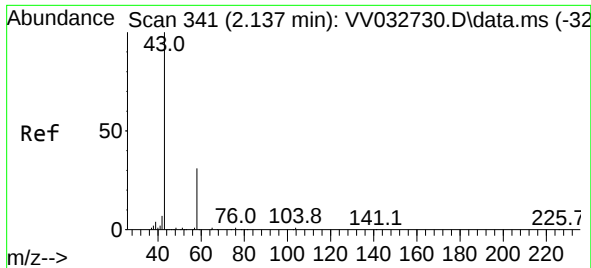

#13

Acetone

Concen: 1.759 ug/L

RT: 2.130 min Scan# 31

Delta R.T. -0.007 min

Lab File: VV032743.D


Acq: 28 Oct 2023 15:41

Instrument :

MSVOA_V

ClientSampleId :

A49H7

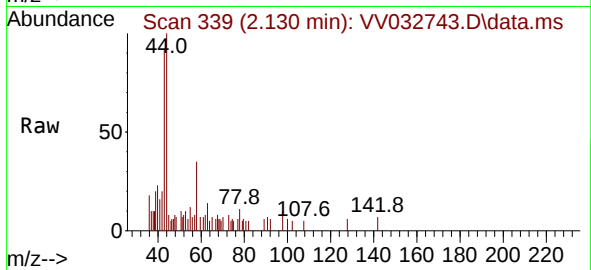

Tgt Ion: 43 Resp: 3971

Ion Ratio Lower Upper

43 100

58 21.0 0.0 50.6

