

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032747.D
 Acq On : 28 Oct 2023 17:19
 Operator : SY/MD
 Sample : 05103-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49W5

Quant Time: Oct 30 01:55:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	130790	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	150262	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	65364	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	47440	4.417	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.400%	
7) Chloroethane-d5	1.532	69	46450	5.089	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	101.800%	
11) 1,1-Dichloroethene-d2	2.060	65	20412	4.234	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	84.600%	
20) 2-Butanone-d5	3.802	46	93549	40.330	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	80.660%	
24) Chloroform-d	4.252	84	88397	4.956	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
26) 1,2-Dichloroethane-d4	4.947	65	45187	5.131	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.600%	
32) Benzene-d6	4.963	84	172954	4.834	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.600%	
36) 1,2-Dichloropropane-d6	5.992	67	55340	5.342	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.800%	
41) Toluene-d8	7.246	98	160432	4.424	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.400%	
43) trans-1,3-Dichloroprop...	7.561	79	18727	4.097	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.030	63	72294	39.905	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.820%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	43798	4.754	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.000%	
66) 1,2-Dichlorobenzene-d4	11.564	152	58710	5.501	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.000%	
Target Compounds						Qvalue
13) Acetone	2.127	43	4280	1.869	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032747.D
Acq On : 28 Oct 2023 17:19
Operator : SY/MD
Sample : 05103-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 79 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49W5

Quant Time: Oct 30 01:55:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

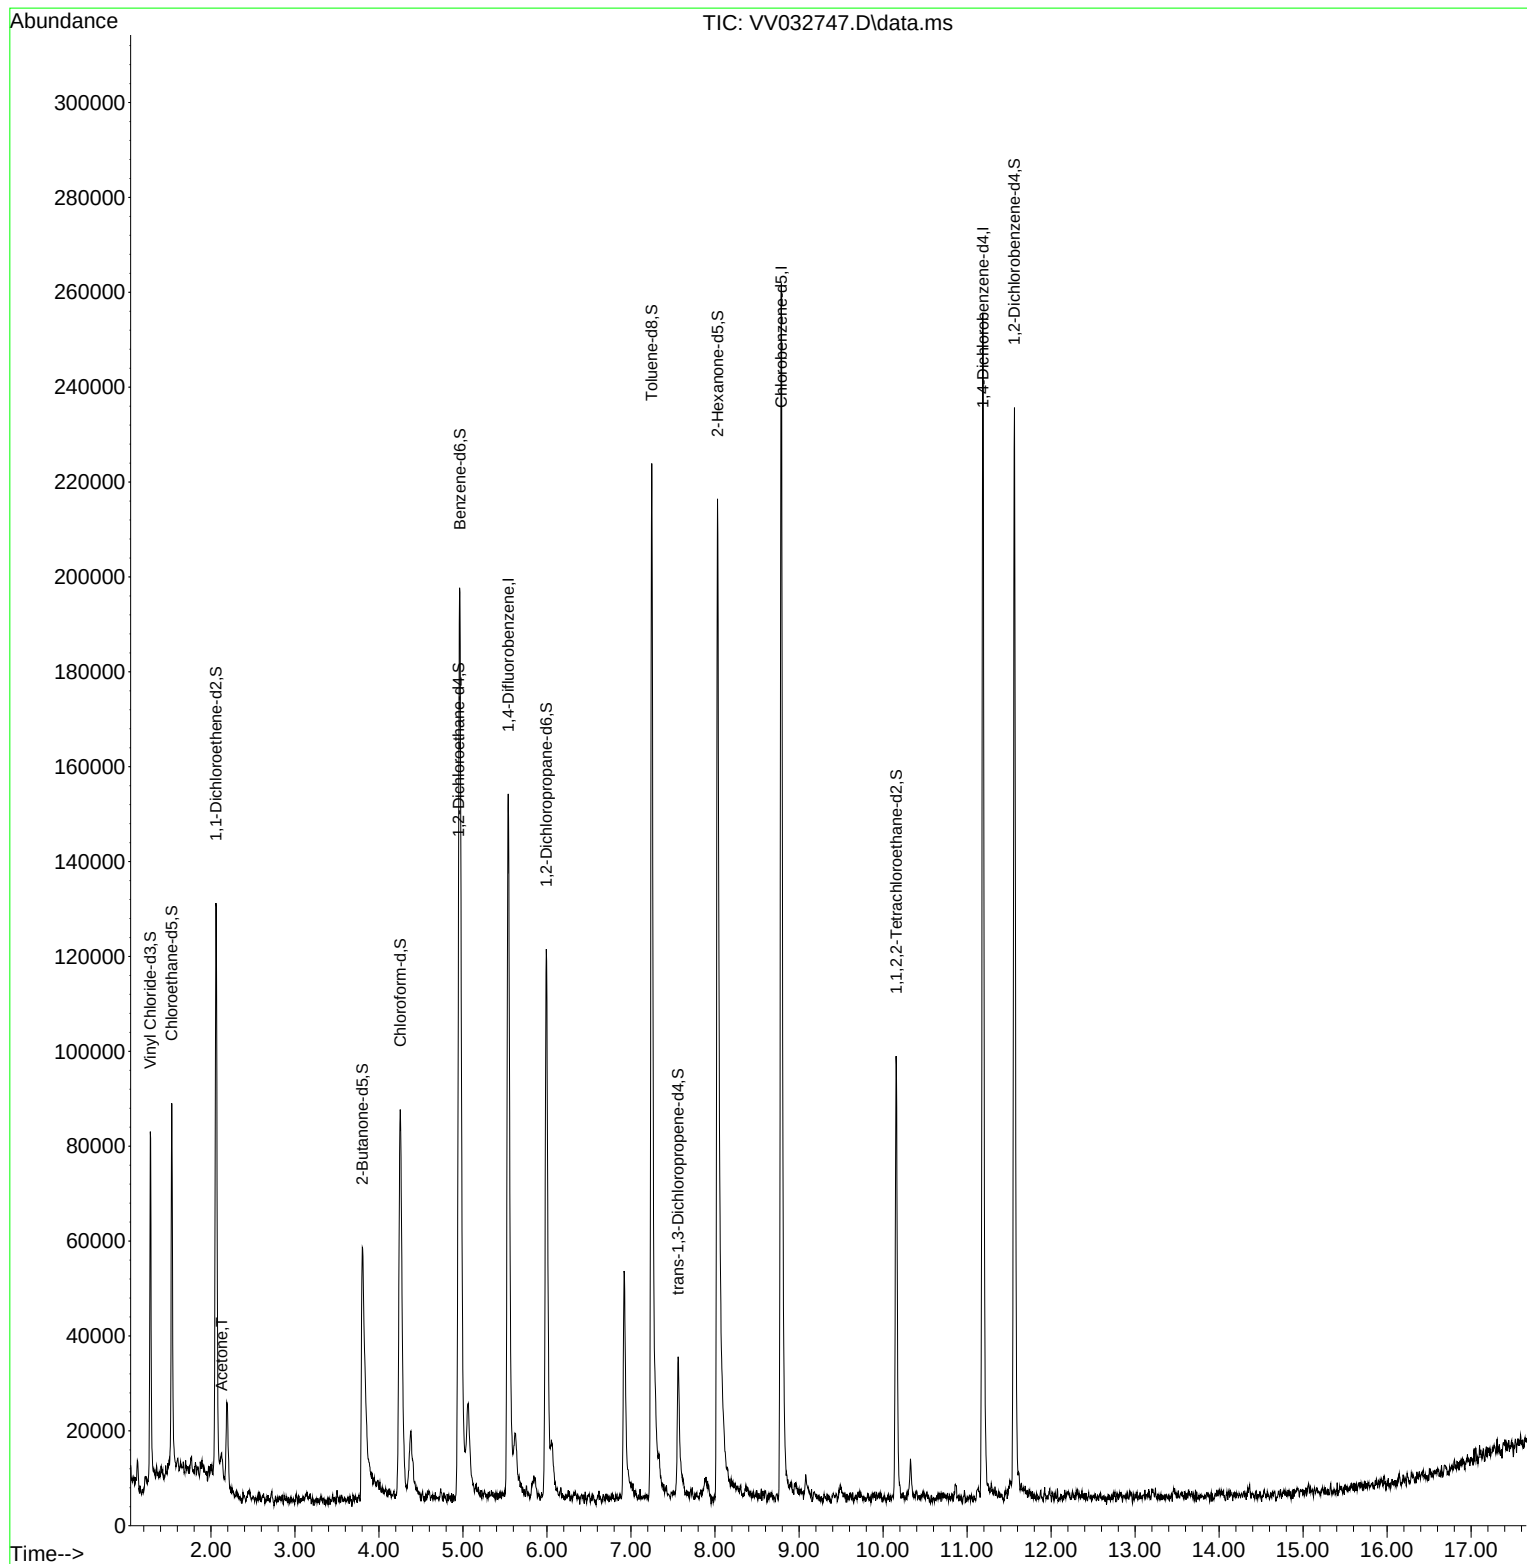

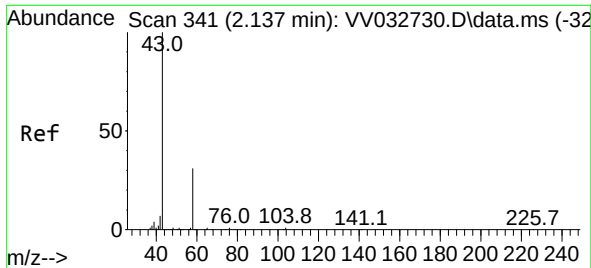

#13

Acetone

Concen: 1.869 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV032747.D

Acq: 28 Oct 2023 17:19

Instrument :

MSVOA_V

ClientSampleId :

A49W5

Tgt Ion: 43 Resp: 4280

Ion Ratio Lower Upper

43 100

58 35.3 0.0 50.6

