

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032748.D
 Acq On : 28 Oct 2023 17:43
 Operator : SY/MD
 Sample : 05103-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49W9

Quant Time: Oct 30 01:55:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	131910	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	154741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	67245	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	49086	4.531	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.600%
7) Chloroethane-d5	1.532	69	46346	5.034	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.600%
11) 1,1-Dichloroethene-d2	2.059	65	19813	4.074	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.400%
20) 2-Butanone-d5	3.799	46	88940	38.018	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.040%
24) Chloroform-d	4.252	84	84240	4.683	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
26) 1,2-Dichloroethane-d4	4.947	65	44116	4.967	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	4.963	84	168446	4.572	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	5.989	67	52549	4.926	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.246	98	159194	4.263	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	7.561	79	19586	4.161	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.200%
46) 2-Hexanone-d5	8.030	63	72814	39.029	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.060%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	42477	4.477	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	58485	5.326	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds					Qvalue	
13) Acetone	2.130	43	4561	1.975	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032748.D
Acq On : 28 Oct 2023 17:43
Operator : SY/MD
Sample : 05103-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49W9

Quant Time: Oct 30 01:55:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

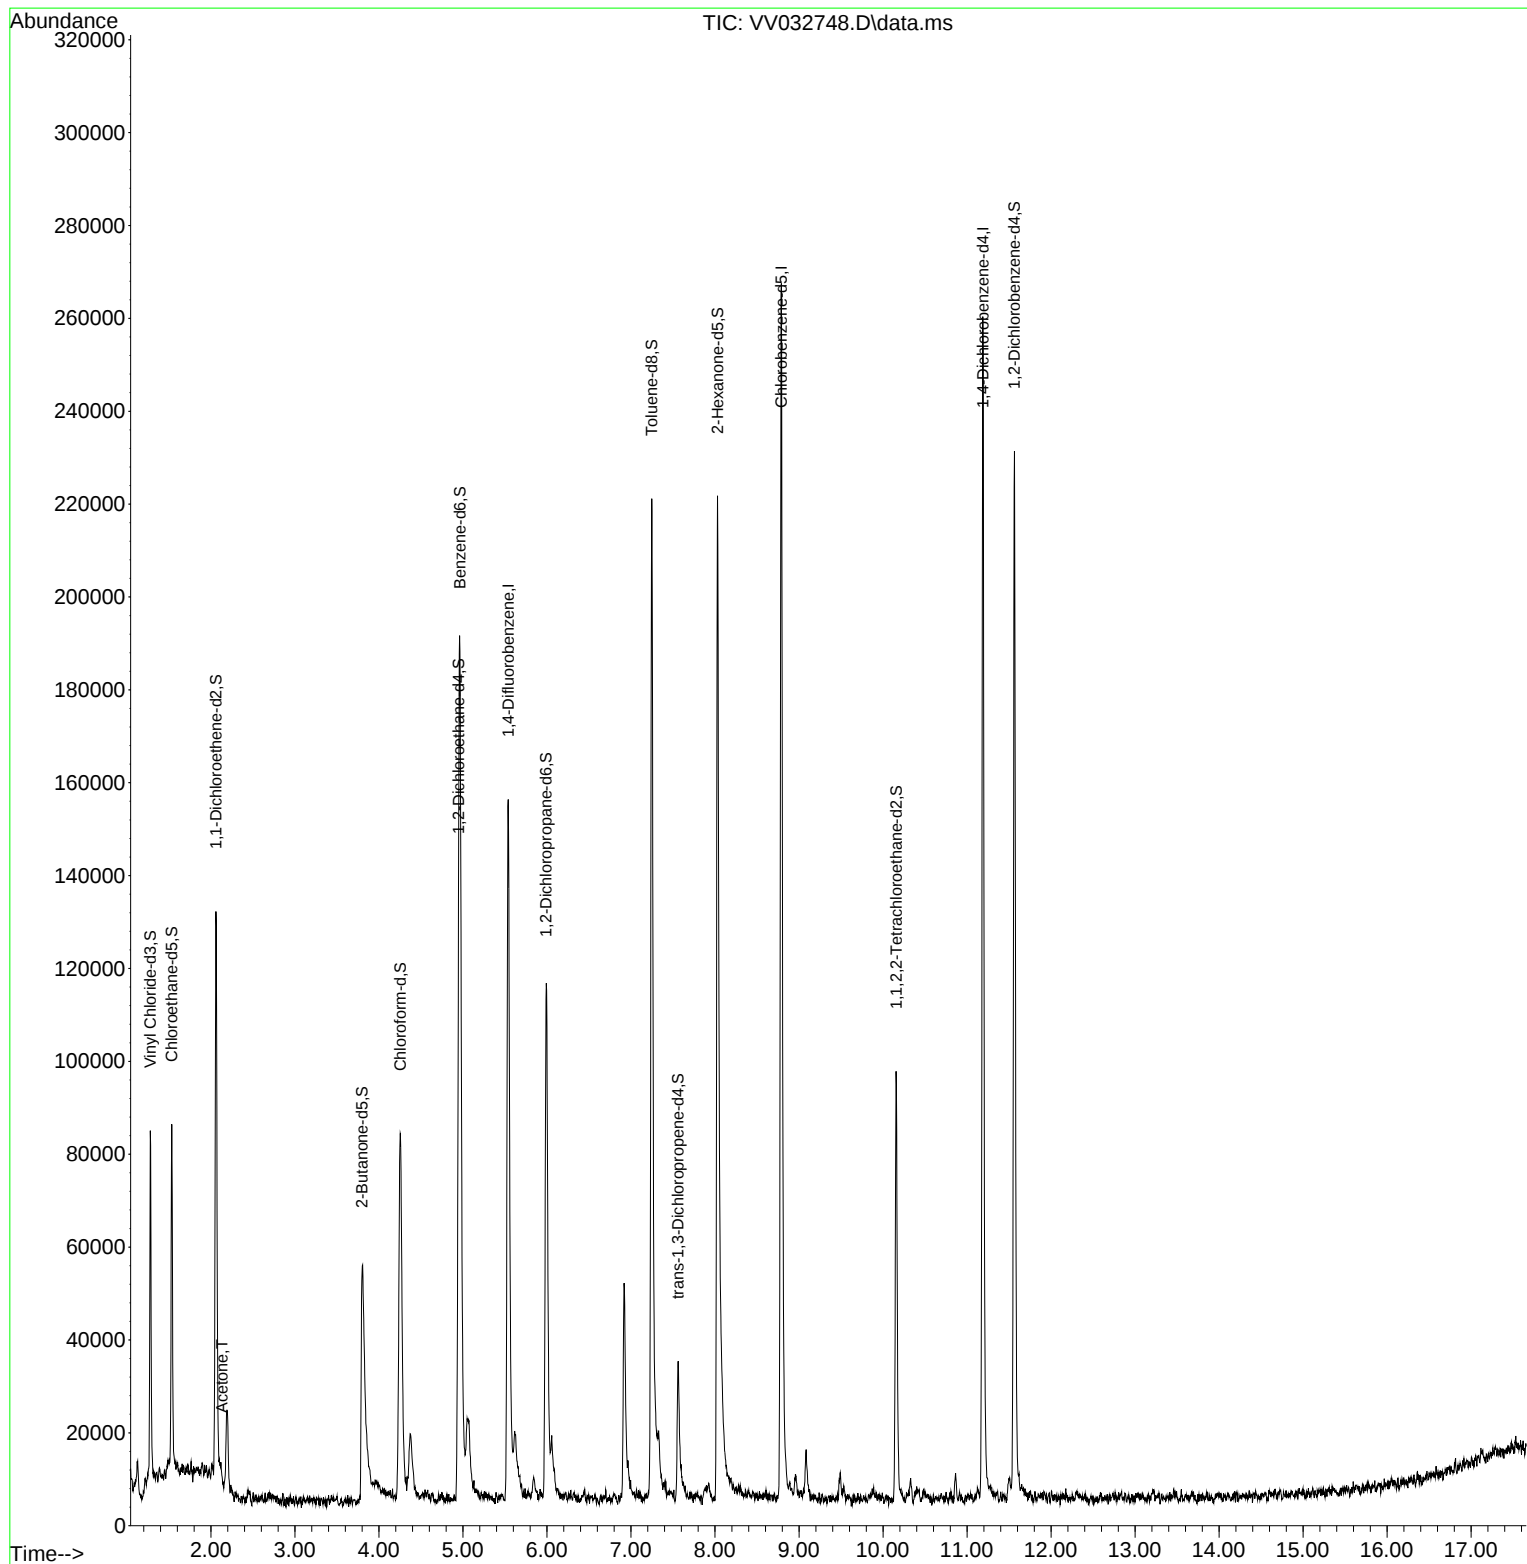

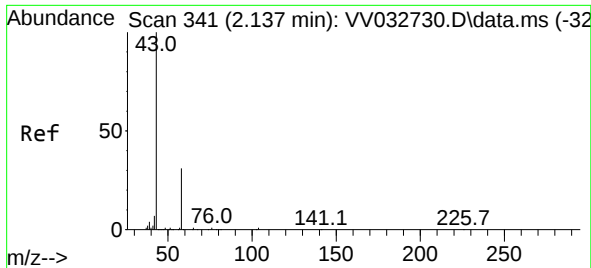

#13

Acetone

Concen: 1.975 ug/L

RT: 2.130 min Scan# 31

Delta R.T. -0.007 min

Lab File: VV032748.D


Acq: 28 Oct 2023 17:43

Instrument :

MSVOA_V

ClientSampleId :

A49W9

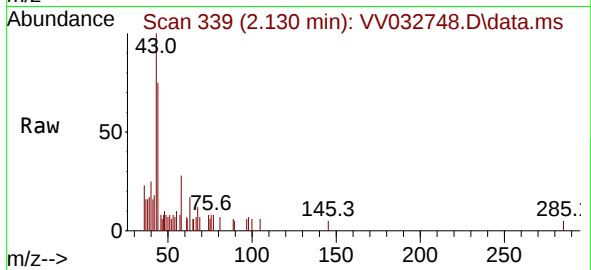

Tgt Ion: 43 Resp: 4561

Ion Ratio Lower Upper

43 100

58 17.9 0.0 50.6

