

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032751.D
 Acq On : 28 Oct 2023 18:56
 Operator : SY/MD
 Sample : 05103-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49X6

Manual Integrations
 APPROVED

Reviewed By : John Carlone 10/30/2023
 Supervised By : Mahesh Dadoda 10/31/2023

Quant Time: Oct 30 01:56:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	129066	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	152398	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	64817	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	47888	4.518	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.400%
7) Chloroethane-d5	1.532	69	48754m	5.412	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.200%
11) 1,1-Dichloroethene-d2	2.060	65	20156	4.236	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.800%
20) 2-Butanone-d5	3.802	46	94847	41.436	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.880%
24) Chloroform-d	4.256	84	89804	5.102	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	4.947	65	44790	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%
32) Benzene-d6	4.963	84	177119	4.881	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	5.992	67	54874	5.223	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.400%
41) Toluene-d8	7.249	98	160522	4.364	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.561	79	20101	4.336	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.030	63	75207	40.931	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.860%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	43743	4.682	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	59280	5.601	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.000%
Target Compounds					Qvalue	
13) Acetone	2.127	43	3794	1.679	ug/L	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032751.D
Acq On : 28 Oct 2023 18:56
Operator : SY/MD
Sample : 05103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
A49X6

Manual Integrations
APPROVED

Reviewed By : John Carlone 10/30/2023
Supervised By : Mahesh Dadoda 10/31/2023

Quant Time: Oct 30 01:56:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

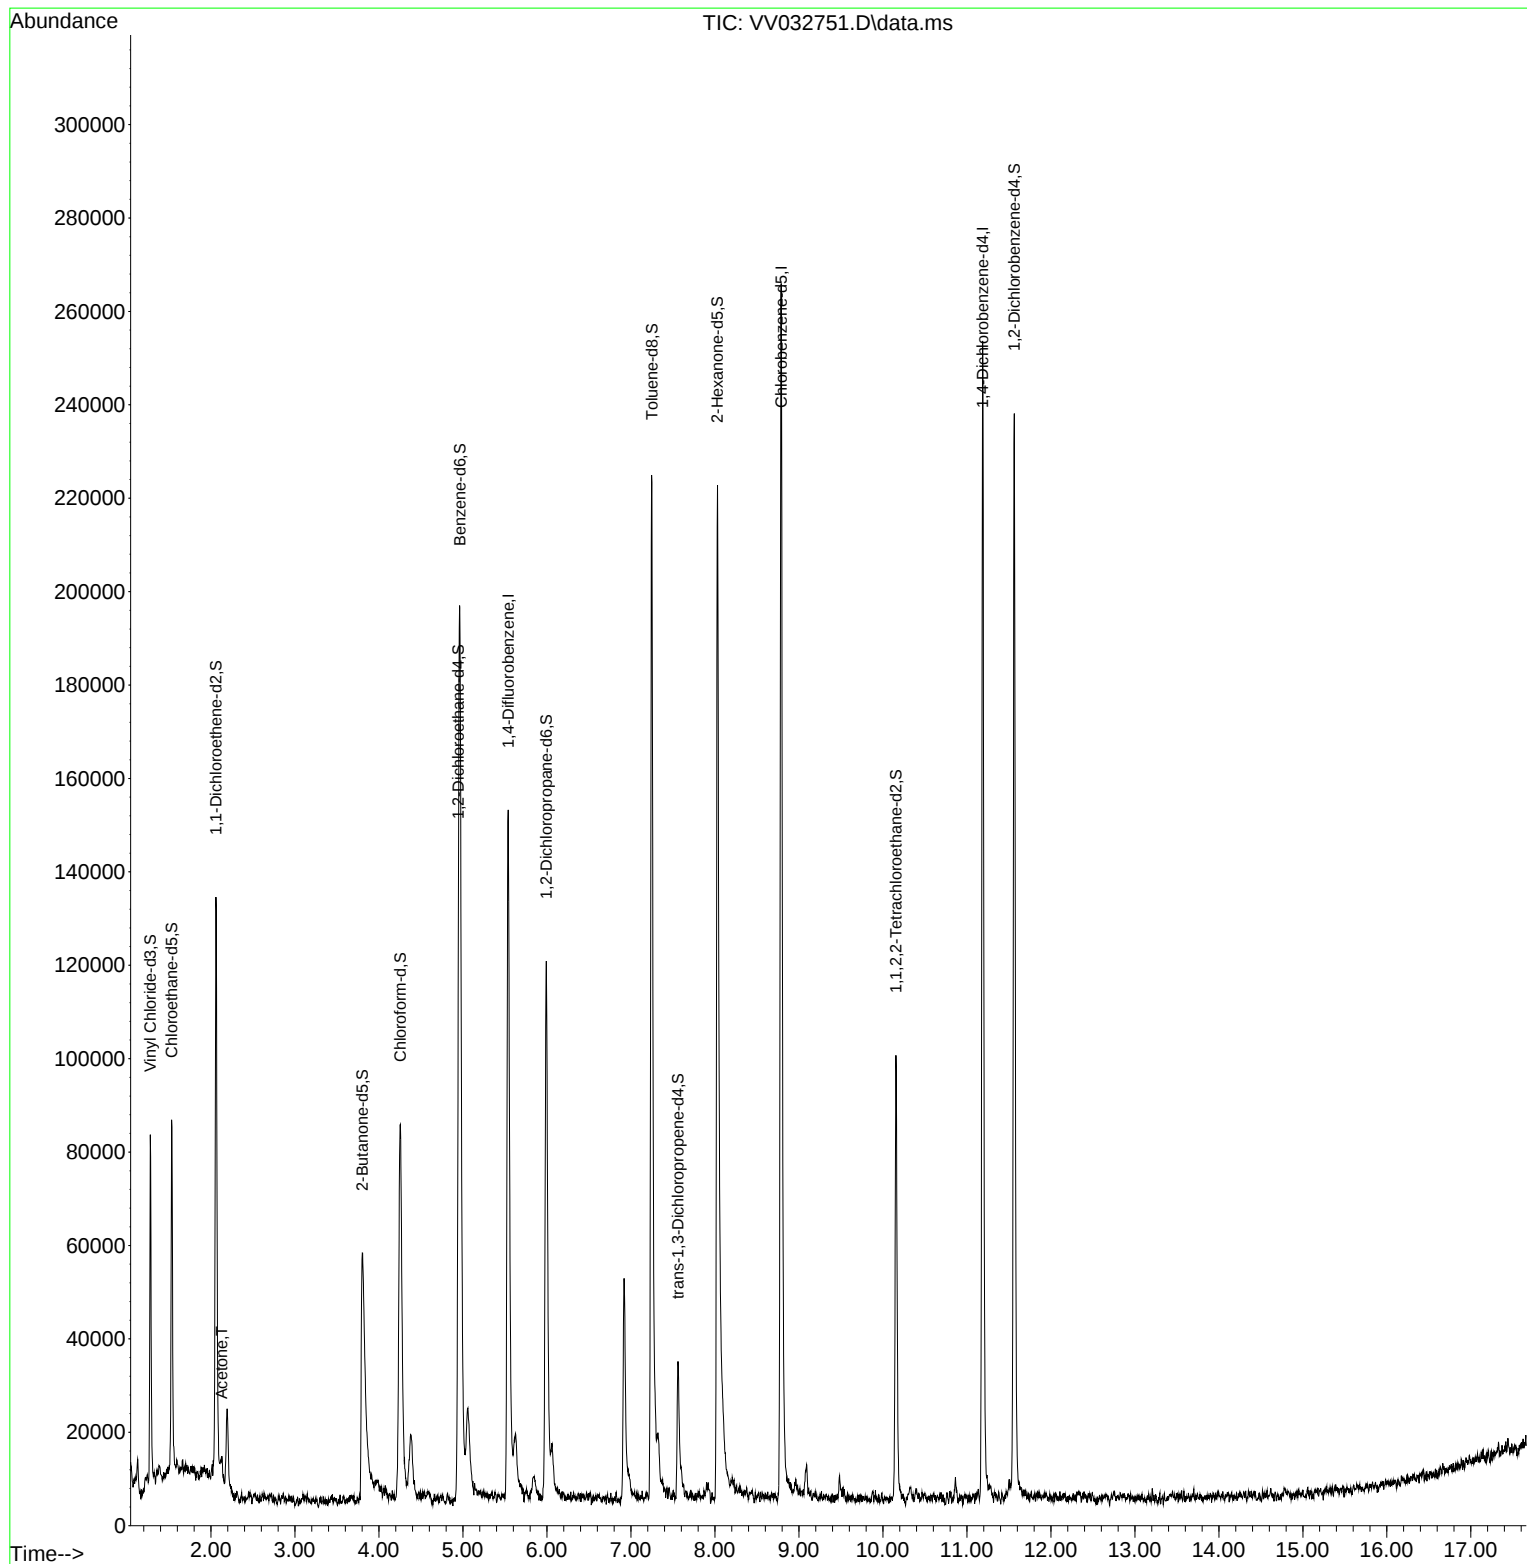

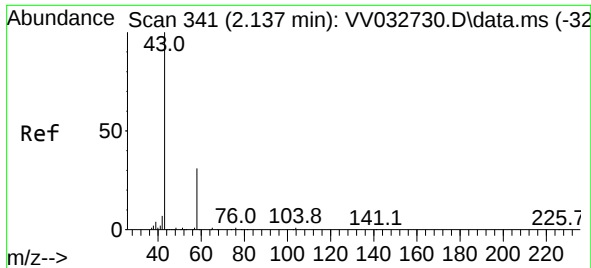

#13

Acetone

Concen: 1.679 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV032751.D


Acq: 28 Oct 2023 18:56

Instrument :

MSVOA_V

ClientSampleId :

A49X6

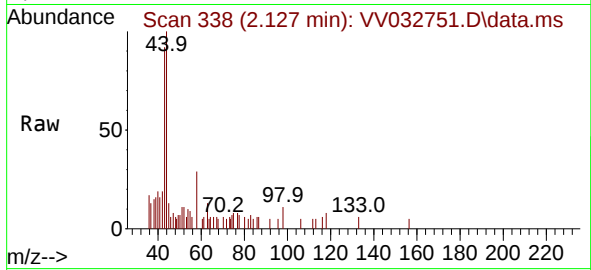

Tgt Ion: 43 Resp: 3794

Ion Ratio Lower Upper

43 100

58 40.5 0.0 50.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 10/30/2023

Supervised By :Mahesh Dadoda 10/31/2023

