

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102723\
 Data File : VW032752.D
 Acq On : 28 Oct 2023 19:21
 Operator : SY/MD
 Sample : 05103-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49X8

Quant Time: Oct 30 03:17:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 01:47:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	126727	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	151328	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	65279	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	48227	4.634	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.600%
7) Chloroethane-d5	1.532	69	48219	5.452	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.000%
11) 1,1-Dichloroethene-d2	2.060	65	20877	4.469	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.400%
20) 2-Butanone-d5	3.802	46	93711	41.695	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.400%
24) Chloroform-d	4.253	84	89197	5.161	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	4.947	65	45619	5.347	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.000%
32) Benzene-d6	4.963	84	175599	4.874	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
36) 1,2-Dichloropropane-d6	5.992	67	54961	5.268	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.400%
41) Toluene-d8	7.246	98	161761	4.429	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.600%
43) trans-1,3-Dichloroprop...	7.561	79	19995	4.343	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.031	63	76204	41.767	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.540%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	45007	4.851	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.000%
66) 1,2-Dichlorobenzene-d4	11.564	152	56999	5.347	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.000%
Target Compounds					Qvalue	
13) Acetone	2.130	43	3482	1.569	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032752.D
Acq On : 28 Oct 2023 19:21
Operator : SY/MD
Sample : 05103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X8

Quant Time: Oct 30 03:17:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 01:47:59 2023
Response via : Initial Calibration

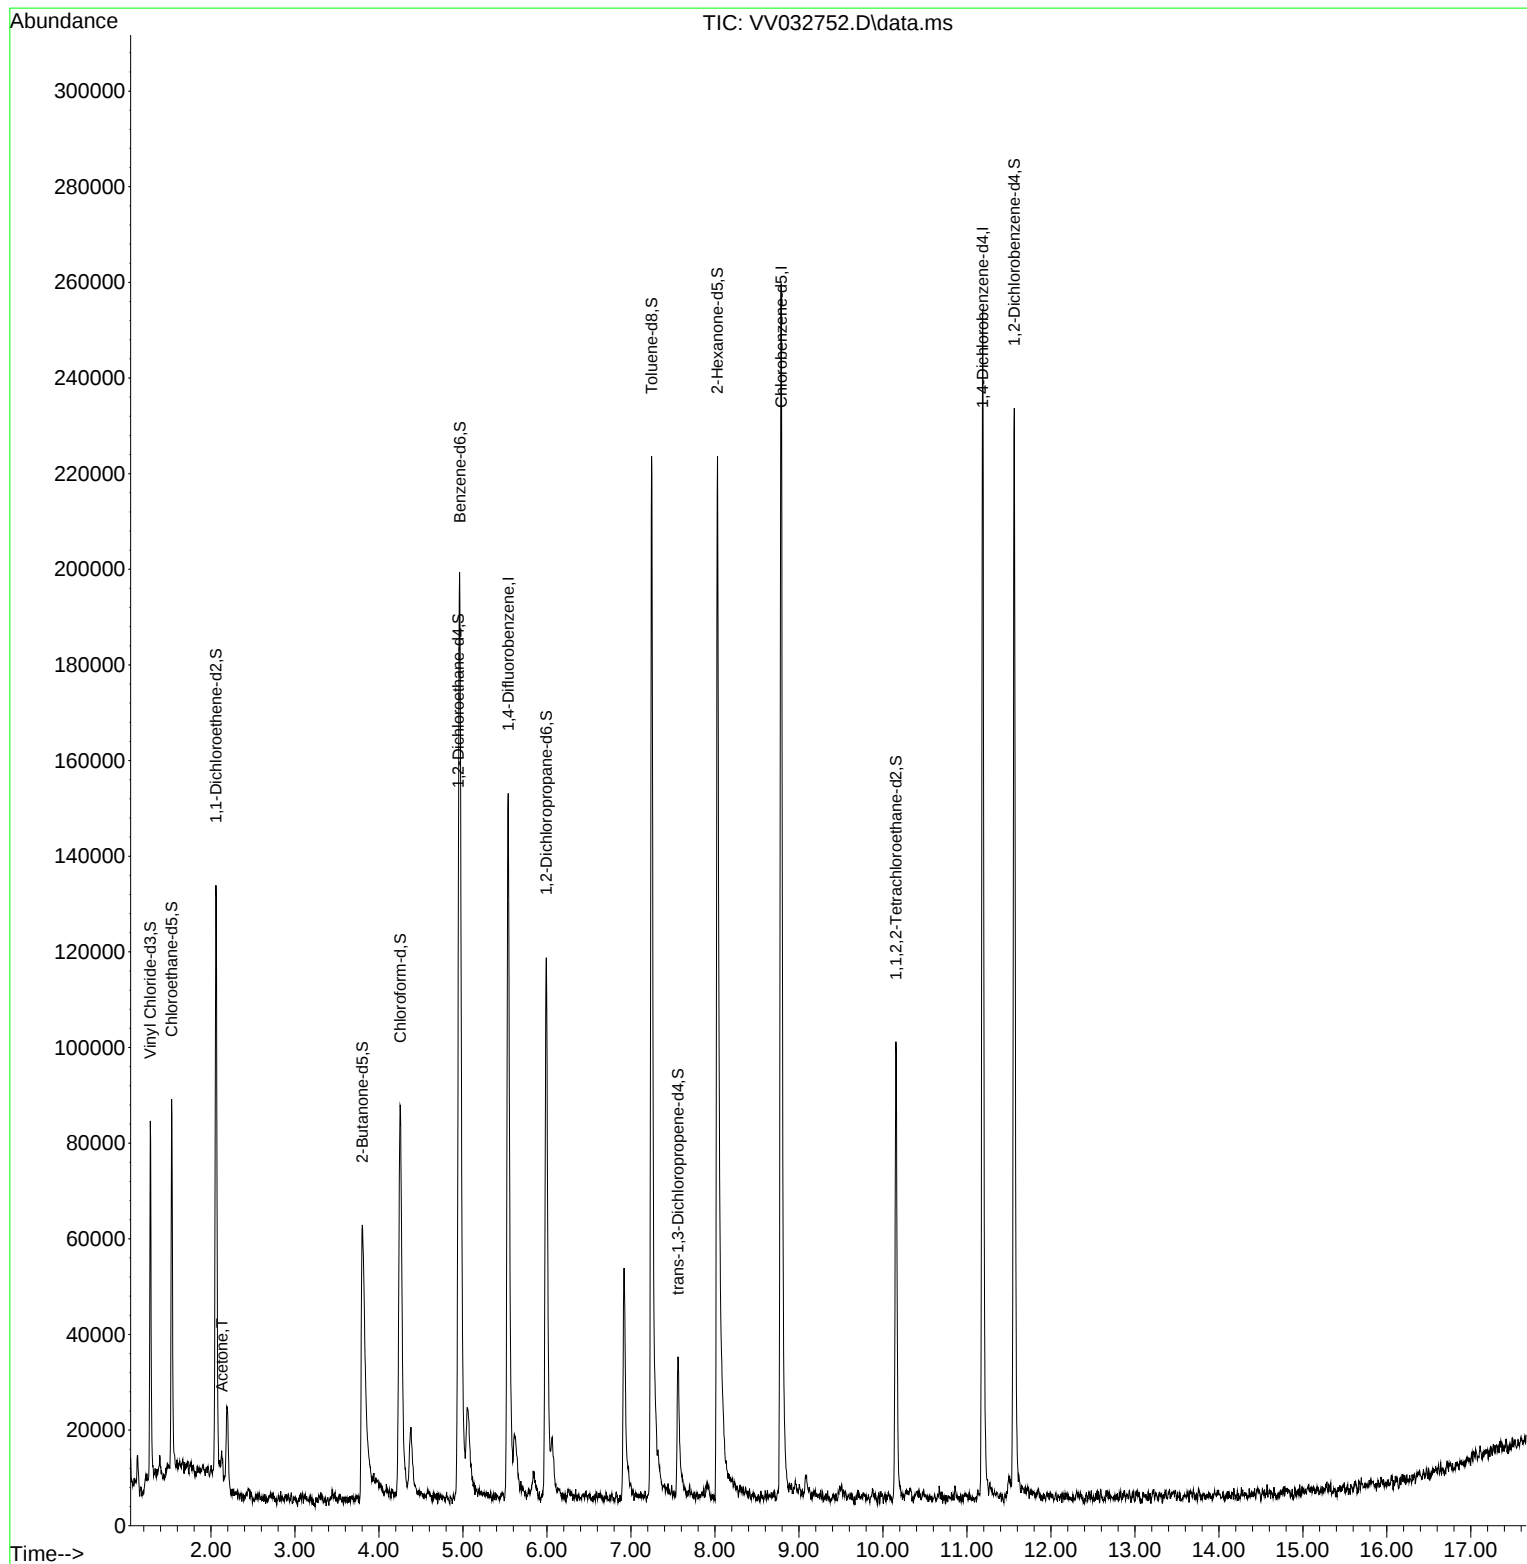

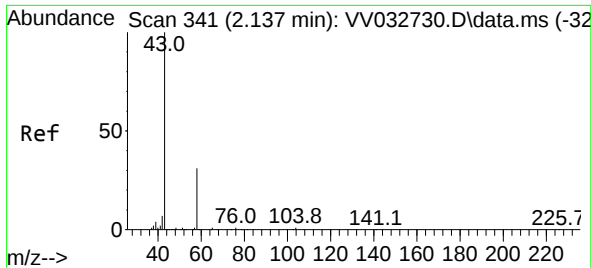

#13

Acetone

Concen: 1.569 ug/L

RT: 2.130 min Scan# 31

Delta R.T. -0.006 min

Lab File: VV032752.D


Acq: 28 Oct 2023 19:21

Instrument :

MSVOA_V

ClientSampleId :

A49X8

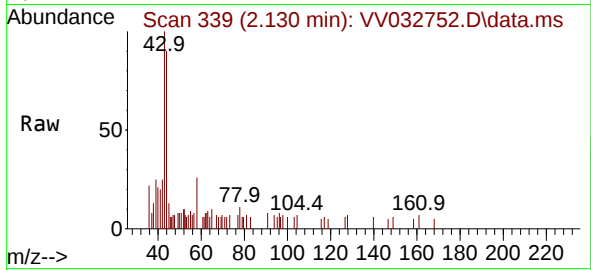

Tgt Ion: 43 Resp: 3482

Ion Ratio Lower Upper

43 100

58 31.2 0.0 50.6

