

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032680.D
 Acq On : 27 Oct 2023 13:40
 Operator : SY/MD
 Sample : VV1027WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK382

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	18	24	33	rVB	9432	14224	2.64%	0.302%
2	1.278	68	74	88	rVB	93356	98469	18.30%	2.090%
3	1.532	147	153	165	rVB	77145	87552	16.28%	1.858%
4	2.060	304	317	330	rBV	140462	211149	39.25%	4.481%
5	2.185	345	356	365	rVB3	19524	34675	6.45%	0.736%
6	2.449	428	438	449	rVB2	17635	30523	5.67%	0.648%
7	2.970	590	600	613	rVV8	11714	21767	4.05%	0.462%
8	3.815	846	863	886	rBV2	30840	119795	22.27%	2.542%
9	4.252	986	999	1019	rBV2	86354	216356	40.22%	4.591%
10	4.368	1027	1035	1045	rVB2	8500	15185	2.82%	0.322%
11	4.960	1200	1219	1238	rBV3	212682	537944	100.00%	11.415%
12	5.539	1388	1399	1416	rBV2	164433	350486	65.15%	7.437%
13	5.992	1529	1540	1556	rBV	119184	251887	46.82%	5.345%
14	6.918	1819	1828	1847	rBV2	55572	118184	21.97%	2.508%
15	7.246	1919	1930	1955	rBV	248738	488102	90.73%	10.358%
16	7.561	2019	2028	2043	rBV2	32638	67268	12.50%	1.427%
17	8.034	2166	2175	2213	rBV	200812	517107	96.13%	10.973%
18	8.789	2400	2410	2429	rBV	270880	487176	90.56%	10.338%
19	10.156	2824	2835	2852	rBV	94734	165978	30.85%	3.522%
20	10.326	2882	2888	2898	rVB7	6446	11831	2.20%	0.251%
21	11.188	3144	3156	3179	rVV	277211	443872	82.51%	9.419%
22	11.564	3260	3273	3285	rBV	242315	389240	72.36%	8.260%
23	12.197	3462	3470	3481	rBV2	5578	9448	1.76%	0.200%
24	13.210	3774	3785	3791	rBV2	5947	10785	2.00%	0.229%
25	13.448	3853	3859	3862	rBV6	6523	7462	1.39%	0.158%
26	13.686	3926	3933	3934	rBV6	6366	5958	1.11%	0.126%




Sum of corrected areas: 4712423

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032680.D
Acq On : 27 Oct 2023 13:40
Operator : SY/MD
Sample : VV1027WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

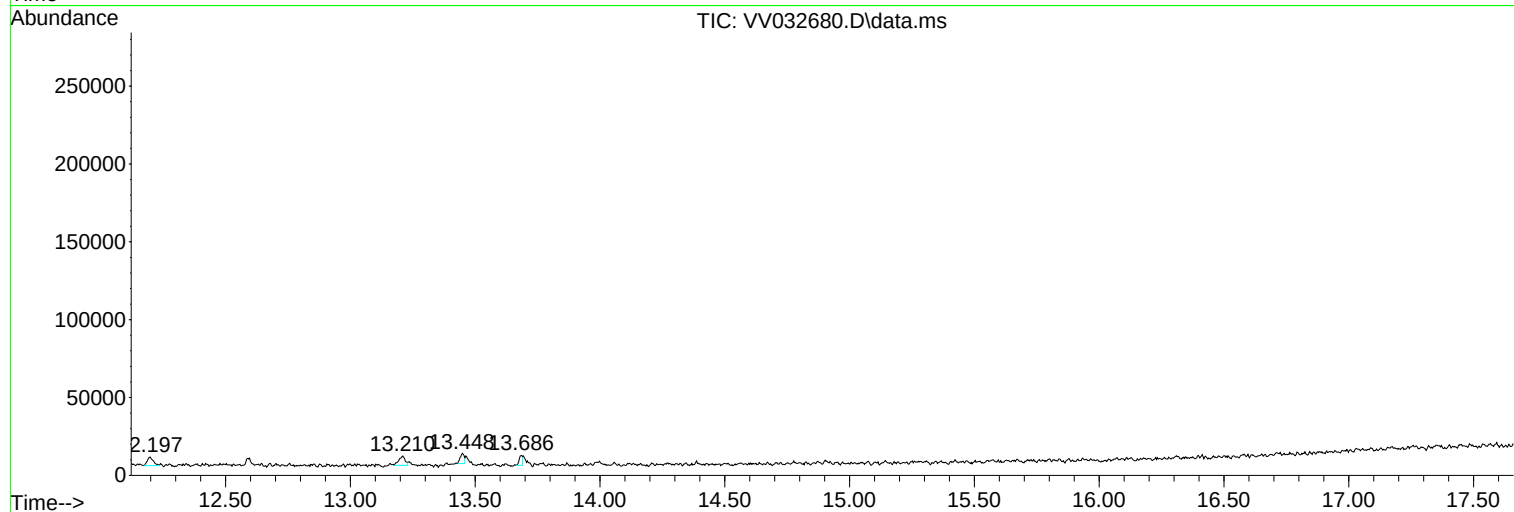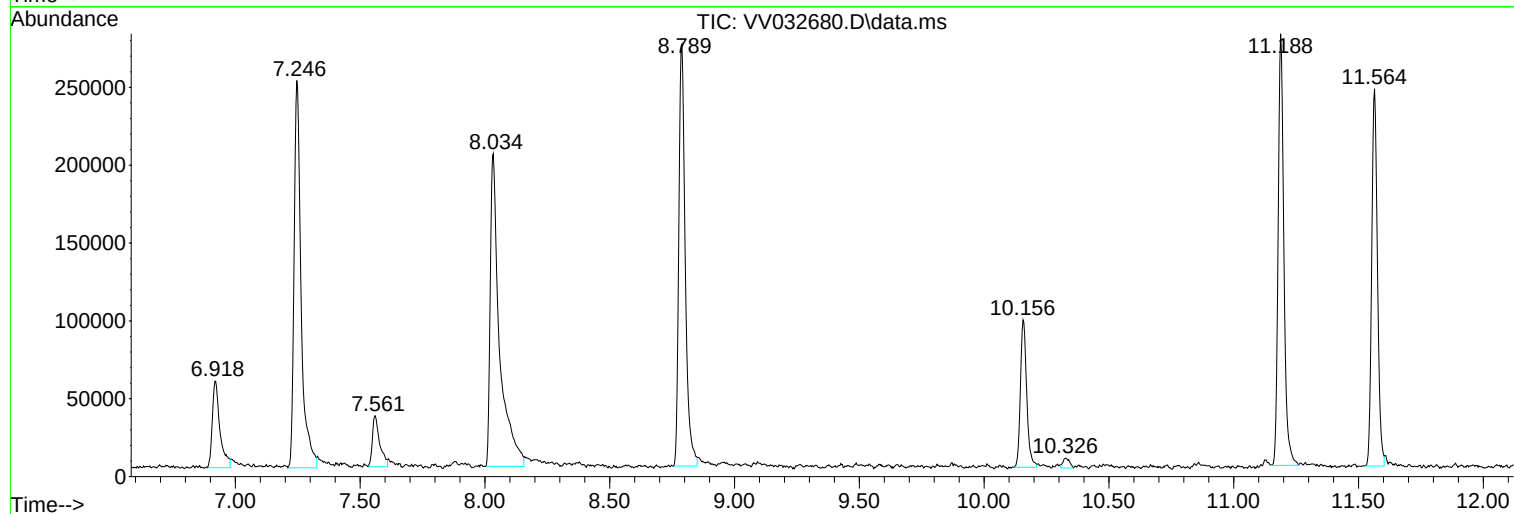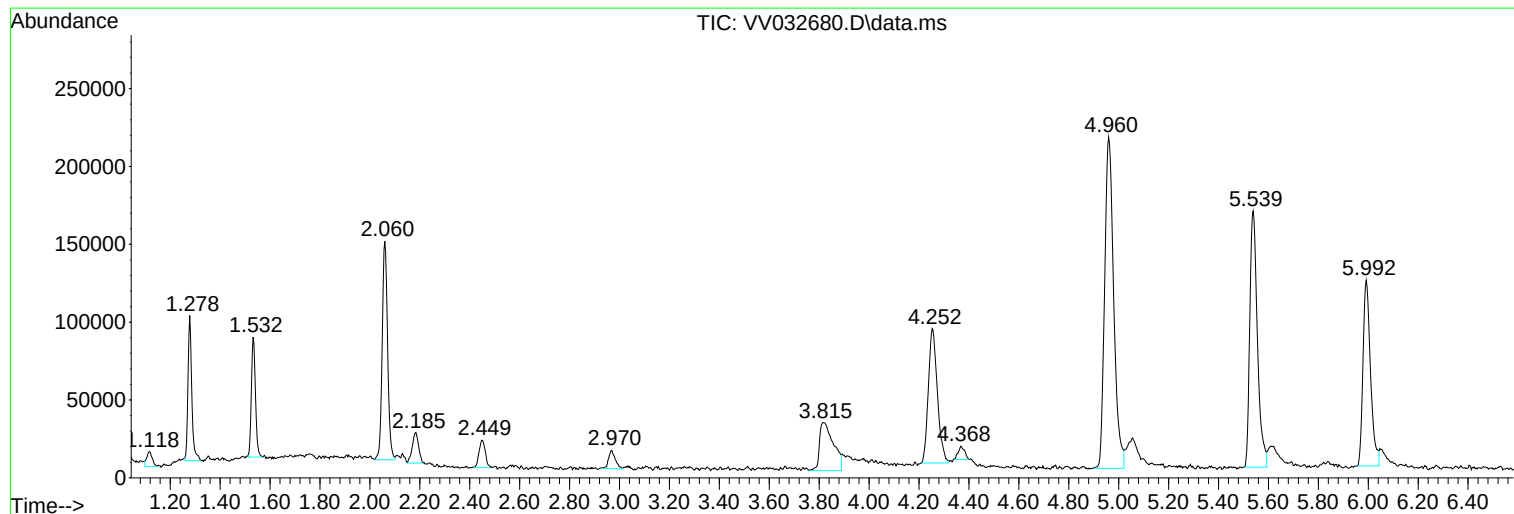

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032680.D
Acq On : 27 Oct 2023 13:40
Operator : SY/MD
Sample : VV1027WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032680.D
Acq On : 27 Oct 2023 13:40
Operator : SY/MD
Sample : VV1027WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc