

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032690.D
 Acq On : 27 Oct 2023 17:43
 Operator : SY/MD
 Sample : 04993-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	88	rVB	80055	95437	16.35%	1.836%
2	1.532	145	153	166	rVV	73140	92381	15.83%	1.777%
3	2.053	306	315	328	rVB	197612	282924	48.48%	5.442%
4	2.442	424	436	449	rBV2	32860	57672	9.88%	1.109%
5	3.828	856	867	895	rBV2	45154	197130	33.78%	3.792%
6	4.253	982	999	1022	rBV	99026	262050	44.90%	5.041%
7	4.957	1202	1218	1237	rBV3	229737	583641	100.00%	11.226%
8	5.535	1385	1398	1414	rBV	181459	378121	64.79%	7.273%
9	5.841	1490	1493	1502	rVB9	4456	5983	1.03%	0.115%
10	5.992	1528	1540	1555	rBV	127630	270644	46.37%	5.206%
11	6.918	1819	1828	1848	rBV	58220	117554	20.14%	2.261%
12	7.246	1919	1930	1952	rBV	265209	490782	84.09%	9.440%
13	7.561	2019	2028	2044	rBV	34121	70795	12.13%	1.362%
14	7.908	2115	2136	2149	rBV3	66203	134395	23.03%	2.585%
15	8.037	2163	2176	2206	rBV	241752	572644	98.12%	11.015%
16	8.789	2399	2410	2430	rBV	289485	496704	85.10%	9.554%
17	10.159	2822	2836	2850	rBV	104294	176853	30.30%	3.402%
18	10.329	2879	2889	2896	rBV6	6777	11968	2.05%	0.230%
19	11.188	3145	3156	3170	rBV	278870	448798	76.90%	8.633%
20	11.564	3260	3273	3288	rBV	262091	422261	72.35%	8.122%
21	13.988	4019	4027	4035	rBV3	7422	12069	2.07%	0.232%
22	15.587	4514	4524	4532	rBV2	10587	18020	3.09%	0.347%




Sum of corrected areas: 5198826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032690.D
Acq On : 27 Oct 2023 17:43
Operator : SY/MD
Sample : 04993-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

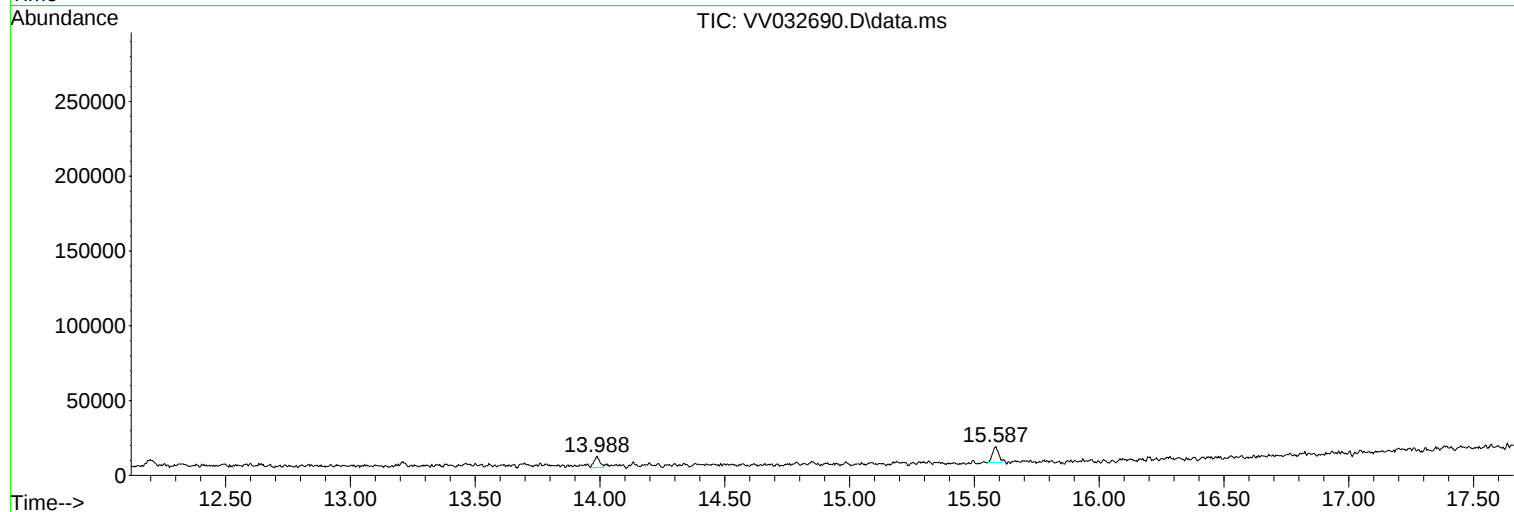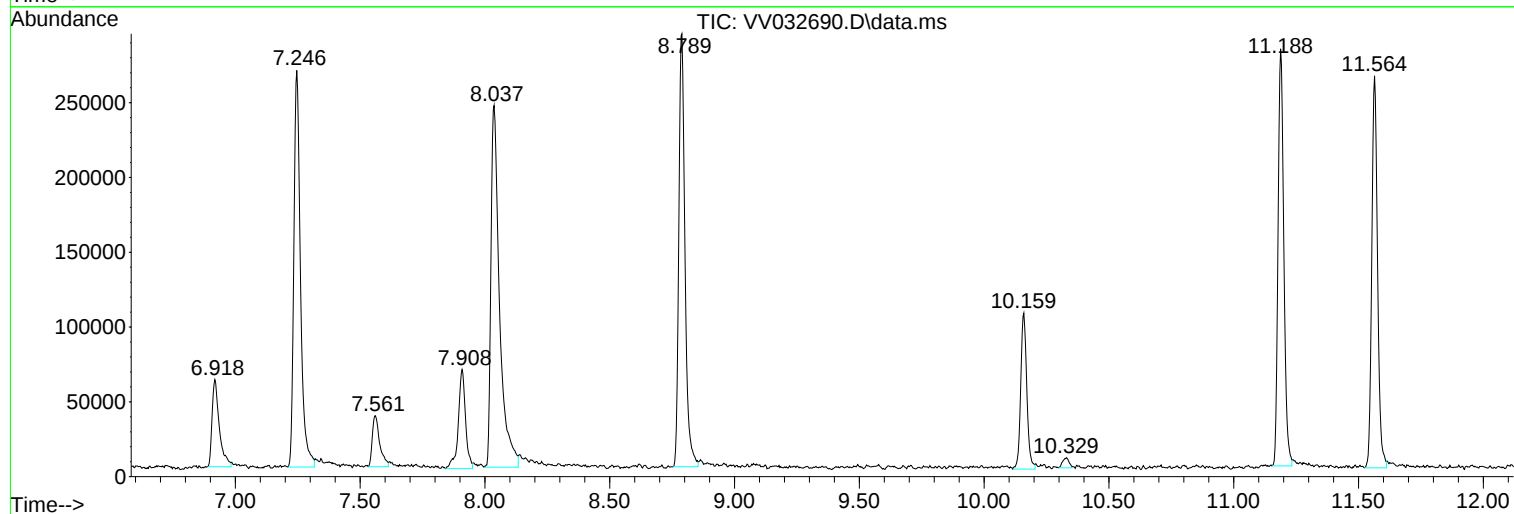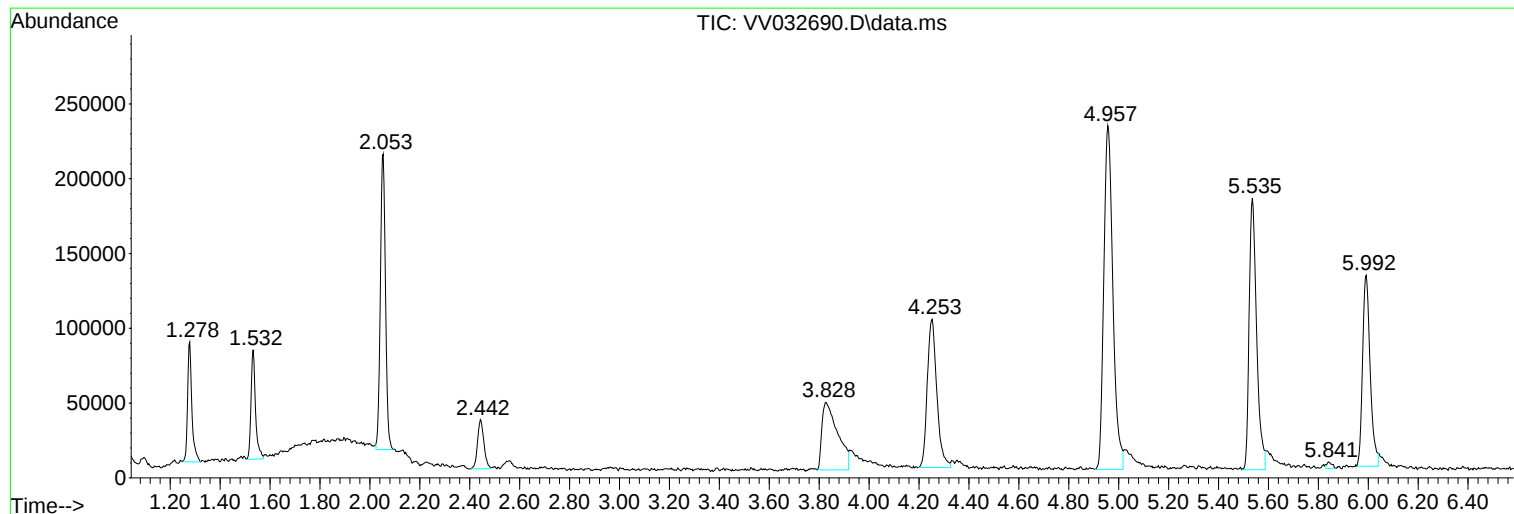

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032690.D
Acq On : 27 Oct 2023 17:43
Operator : SY/MD
Sample : 04993-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032690.D
Acq On : 27 Oct 2023 17:43
Operator : SY/MD
Sample : 04993-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc