

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032693.D
 Acq On : 27 Oct 2023 18:56
 Operator : SY/MD
 Sample : 05055-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48Z9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	18	24	32	rVB2	5285	8248	1.54%	0.166%
2	1.217	50	55	61	rBV	9989	13084	2.44%	0.264%
3	1.278	68	74	84	rBV	87847	91730	17.08%	1.851%
4	1.532	147	153	163	rBV	78279	90057	16.77%	1.818%
5	2.059	308	317	332	rVV	130311	194436	36.21%	3.924%
6	2.185	346	356	370	rVB2	19191	37682	7.02%	0.761%
7	3.805	851	860	886	rBV2	53104	175093	32.60%	3.534%
8	4.252	984	999	1023	rBV	87778	230345	42.89%	4.649%
9	4.375	1025	1037	1054	rVB3	13463	38699	7.21%	0.781%
10	4.960	1204	1219	1238	rBV2	208175	537040	100.00%	10.839%
11	5.538	1385	1399	1415	rBV	162653	341837	63.65%	6.899%
12	5.992	1527	1540	1555	rBV2	121347	261898	48.77%	5.286%
13	6.918	1818	1828	1841	rBV2	53631	106408	19.81%	2.148%
14	7.246	1919	1930	1946	rBV	245181	458464	85.37%	9.253%
15	7.323	1946	1954	1978	rVB	55152	121173	22.56%	2.446%
16	7.561	2017	2028	2044	rBV2	33062	72534	13.51%	1.464%
17	8.030	2163	2174	2200	rBV	240897	514179	95.74%	10.377%
18	8.789	2399	2410	2430	rBV	269355	476815	88.79%	9.623%
19	8.953	2453	2461	2471	rBV	14218	24552	4.57%	0.496%
20	9.079	2490	2500	2516	rBV	36639	73020	13.60%	1.474%
21	9.484	2616	2626	2637	rBV2	15657	29528	5.50%	0.596%
22	10.156	2822	2835	2849	rBV	99311	167236	31.14%	3.375%
23	10.329	2882	2889	2899	rVB5	9172	15116	2.81%	0.305%
24	10.390	2899	2908	2914	rBV4	8765	14511	2.70%	0.293%
25	10.857	3044	3053	3067	rBV3	13589	24927	4.64%	0.503%
26	11.188	3145	3156	3173	rBV	269656	429835	80.04%	8.675%
27	11.278	3182	3184	3193	rVB10	4788	5443	1.01%	0.110%
28	11.564	3262	3273	3289	rBV	250528	400875	74.65%	8.091%




Sum of corrected areas: 4954765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032693.D
Acq On : 27 Oct 2023 18:56
Operator : SY/MD
Sample : 05055-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48Z9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

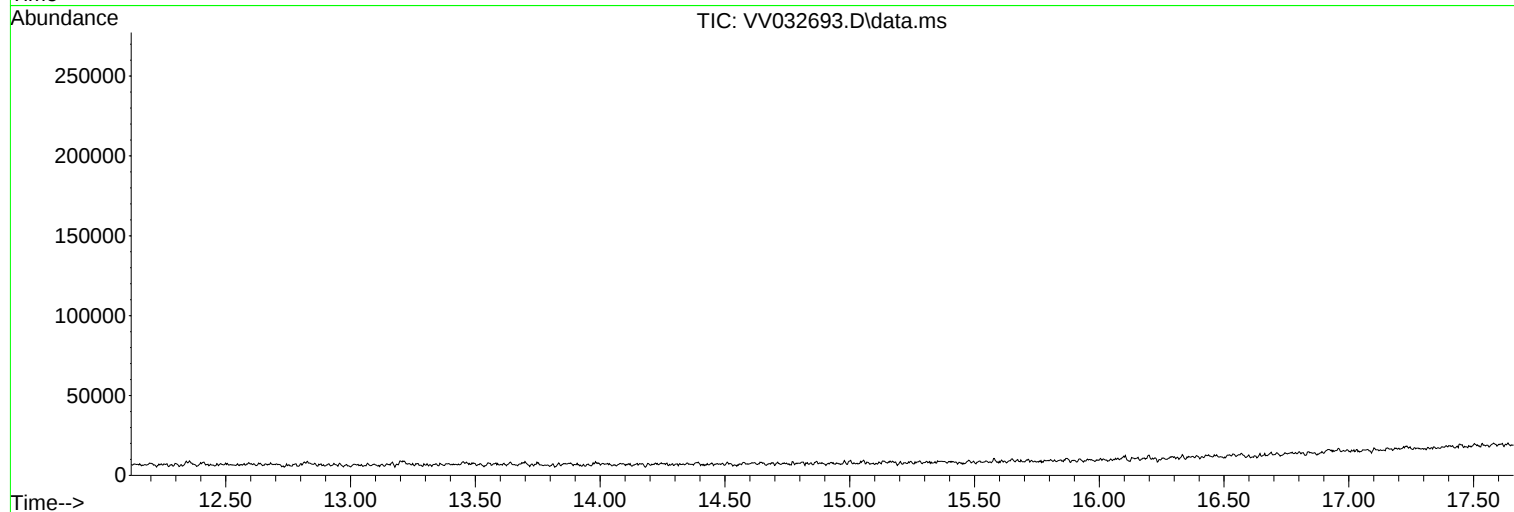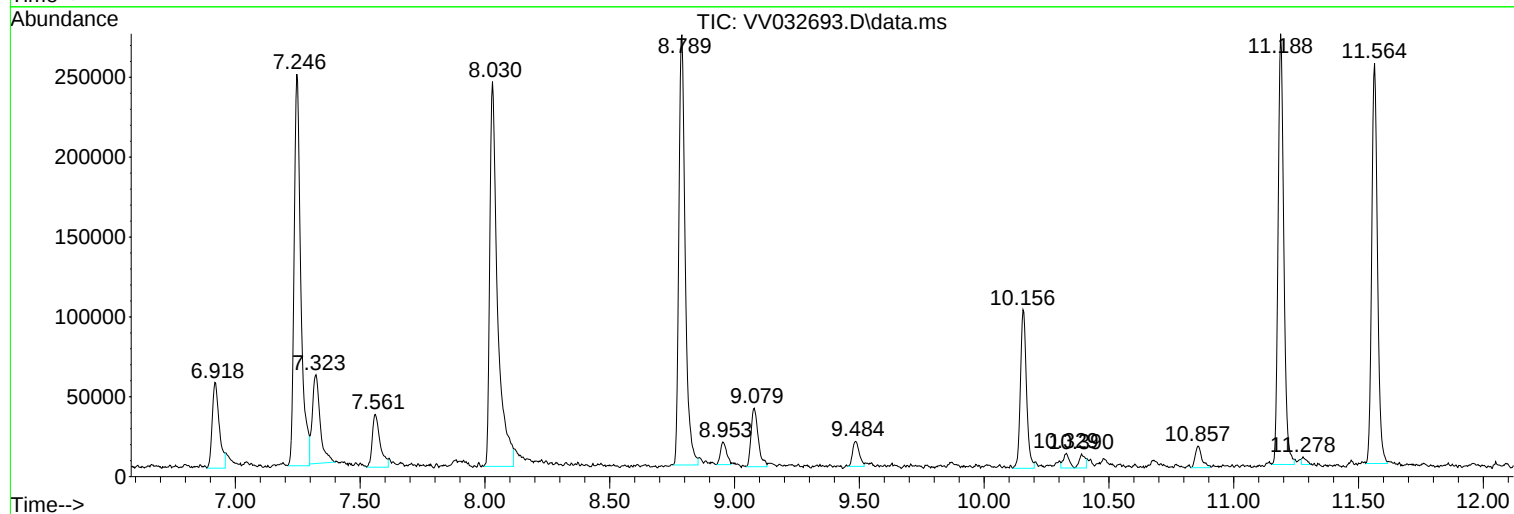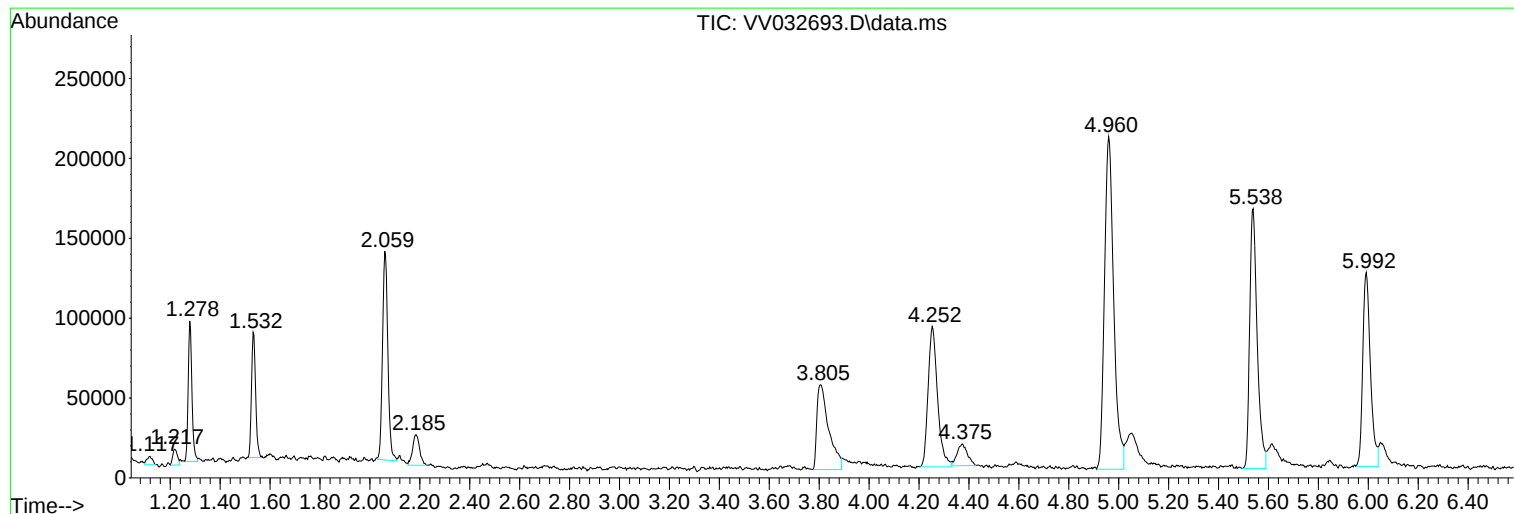

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032693.D
Acq On : 27 Oct 2023 18:56
Operator : SY/MD
Sample : 05055-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48Z9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032693.D
Acq On : 27 Oct 2023 18:56
Operator : SY/MD
Sample : 05055-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48Z9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------