

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032695.D
 Acq On : 27 Oct 2023 19:45
 Operator : SY/MD
 Sample : 05055-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4907

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	19	25	36	rVB	8531	14579	2.83%	0.319%
2	1.217	50	55	63	rBV	13215	18052	3.51%	0.395%
3	1.278	68	74	82	rVV	80607	84238	16.37%	1.845%
4	1.388	103	108	114	rVB2	4196	5382	1.05%	0.118%
5	1.532	146	153	166	rBV	75277	88251	17.15%	1.933%
6	2.060	309	317	329	rBV	125789	181692	35.30%	3.980%
7	2.188	347	357	367	rVB2	18537	35005	6.80%	0.767%
8	3.806	850	860	886	rBV2	58857	198547	38.58%	4.349%
9	4.256	983	1000	1017	rBV2	87202	225539	43.82%	4.940%
10	4.375	1028	1037	1044	rBV2	8717	17504	3.40%	0.383%
11	4.960	1203	1219	1239	rBV3	201589	514651	100.00%	11.272%
12	5.060	1242	1250	1268	rVB5	16131	47467	9.22%	1.040%
13	5.539	1388	1399	1417	rBV	153947	322230	62.61%	7.058%
14	5.992	1526	1540	1554	rBV	118459	246564	47.91%	5.400%
15	6.918	1819	1828	1842	rBV2	51344	102959	20.01%	2.255%
16	7.246	1917	1930	1953	rBV	231658	451752	87.78%	9.895%
17	7.561	2018	2028	2043	rBV2	31429	66414	12.90%	1.455%
18	7.883	2116	2128	2131	rBV10	6118	10504	2.04%	0.230%
19	8.030	2165	2174	2210	rBV	217427	498971	96.95%	10.929%
20	8.789	2397	2410	2431	rBV	263655	468435	91.02%	10.260%
21	10.156	2823	2835	2847	rBV	93636	150733	29.29%	3.301%
22	10.326	2878	2888	2898	rBV8	7659	14414	2.80%	0.316%
23	11.188	3145	3156	3174	rBV	255150	413802	80.40%	9.063%
24	11.497	3244	3252	3254	rBV8	8104	9680	1.88%	0.212%
25	11.564	3261	3273	3291	rVB	229711	372762	72.43%	8.165%
26	12.201	3462	3471	3476	rBV10	3926	5465	1.06%	0.120%




Sum of corrected areas: 4565592

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032695.D
Acq On : 27 Oct 2023 19:45
Operator : SY/MD
Sample : 05055-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4907

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

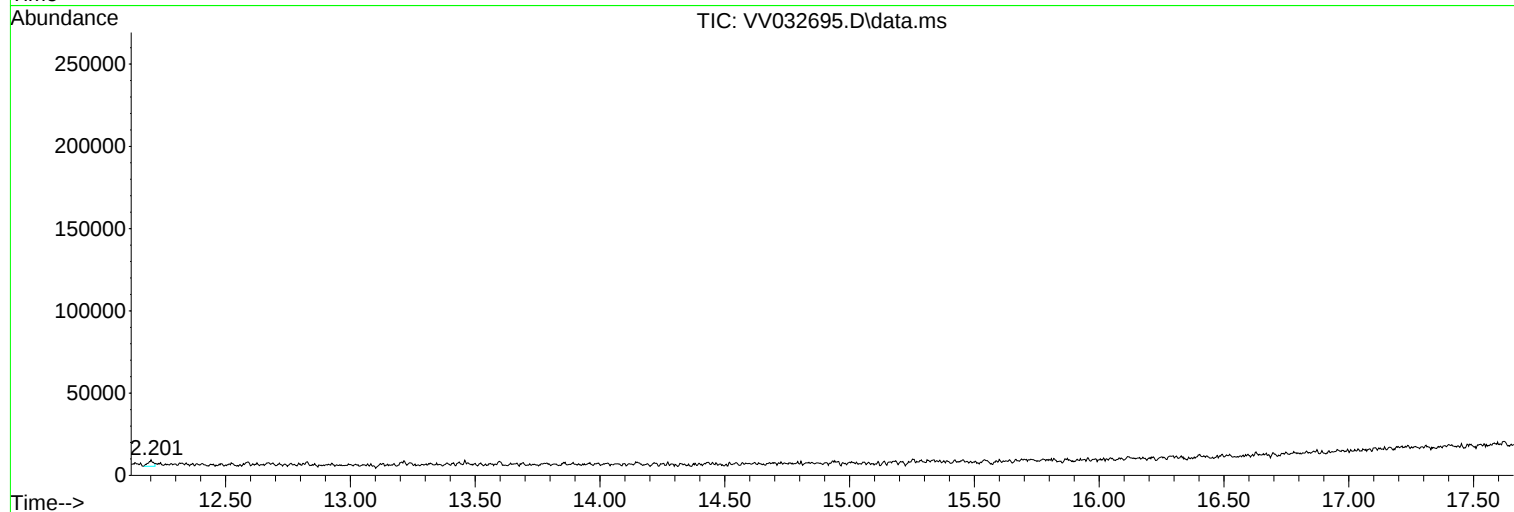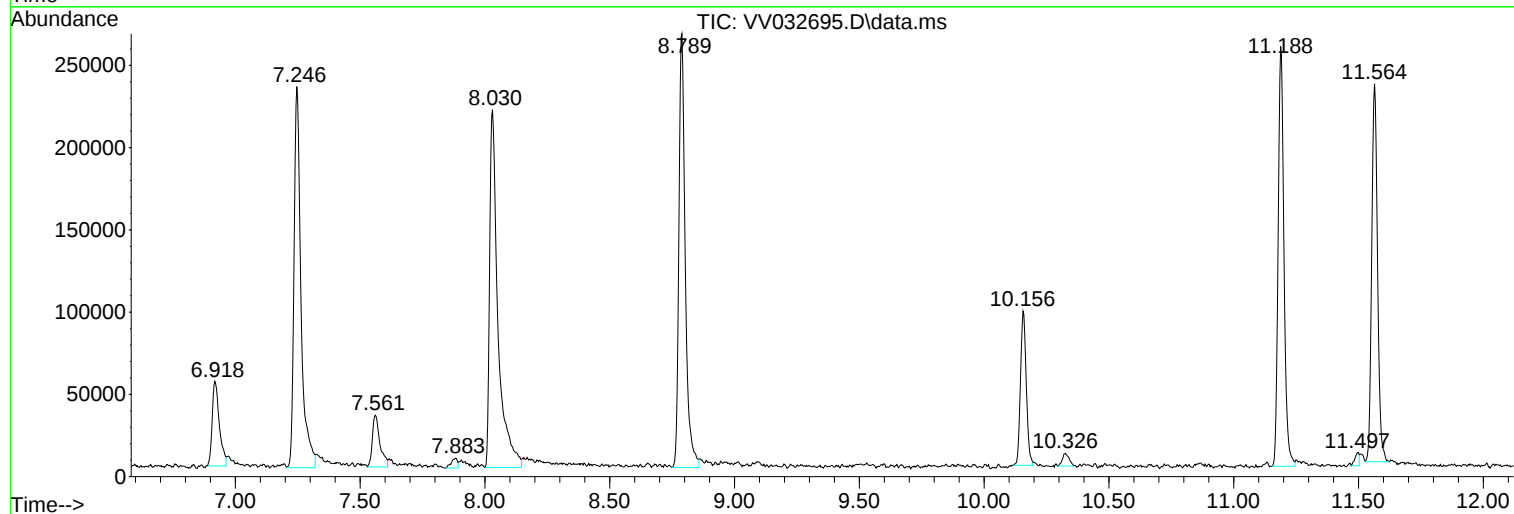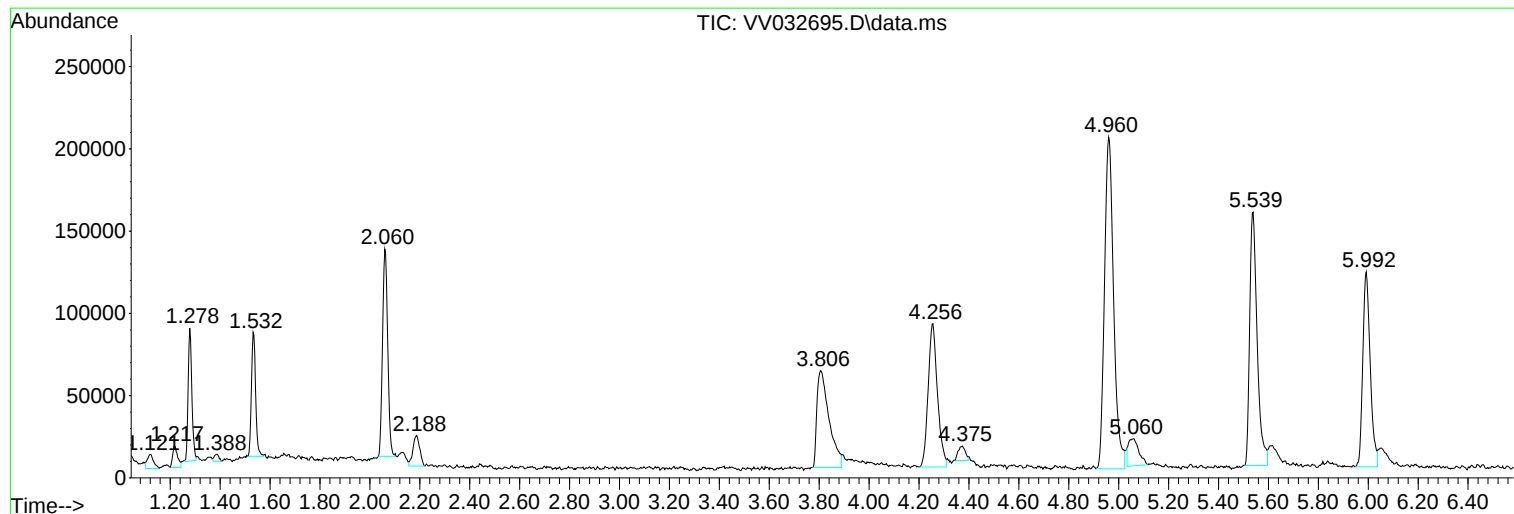

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032695.D
Acq On : 27 Oct 2023 19:45
Operator : SY/MD
Sample : 05055-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4907

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032695.D
Acq On : 27 Oct 2023 19:45
Operator : SY/MD
Sample : 05055-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4907

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc