

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032696.D
 Acq On : 27 Oct 2023 20:09
 Operator : SY/MD
 Sample : 05055-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4939

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	18	24	28	rVB2	5154	5767	1.11%	0.126%
2	1.217	48	55	64	rBV	22462	28644	5.51%	0.626%
3	1.278	66	74	86	rVB	81019	90428	17.39%	1.976%
4	1.532	147	153	166	rVB	79819	92687	17.82%	2.025%
5	2.060	307	317	329	rBV	130003	189149	36.37%	4.133%
6	2.185	348	356	368	rVB2	16854	30100	5.79%	0.658%
7	3.802	850	859	884	rBV	54929	170659	32.81%	3.729%
8	4.253	984	999	1021	rBV2	86129	230386	44.29%	5.034%
9	4.372	1026	1036	1058	rVB4	12243	36866	7.09%	0.805%
10	4.960	1202	1219	1237	rBV3	205505	520118	100.00%	11.364%
11	5.056	1243	1249	1265	rVB5	15858	36799	7.08%	0.804%
12	5.539	1386	1399	1416	rBV	155789	332883	64.00%	7.273%
13	5.992	1526	1540	1554	rBV	118773	248962	47.87%	5.440%
14	6.918	1819	1828	1842	rBV	52431	102366	19.68%	2.237%
15	7.246	1919	1930	1953	rBV	236815	451525	86.81%	9.865%
16	7.561	2018	2028	2041	rBV	32296	61493	11.82%	1.344%
17	8.031	2162	2174	2206	rBV	224514	501859	96.49%	10.965%
18	8.789	2398	2410	2432	rBV	275860	481517	92.58%	10.521%
19	10.156	2822	2835	2854	rBV	92612	153342	29.48%	3.350%
20	10.323	2878	2887	2898	rVB	5506	11337	2.18%	0.248%
21	11.188	3145	3156	3176	rBV	264091	421480	81.04%	9.209%
22	11.564	3262	3273	3292	rVB	236013	378465	72.77%	8.269%




Sum of corrected areas: 4576832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032696.D
Acq On : 27 Oct 2023 20:09
Operator : SY/MD
Sample : 05055-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4939

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

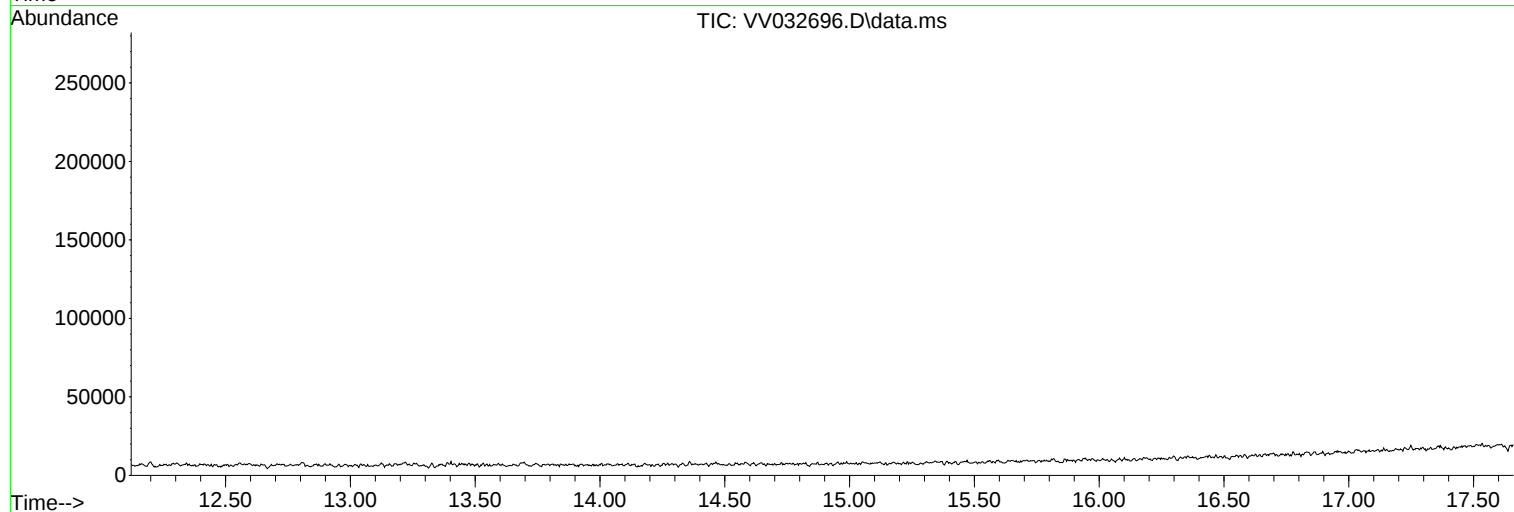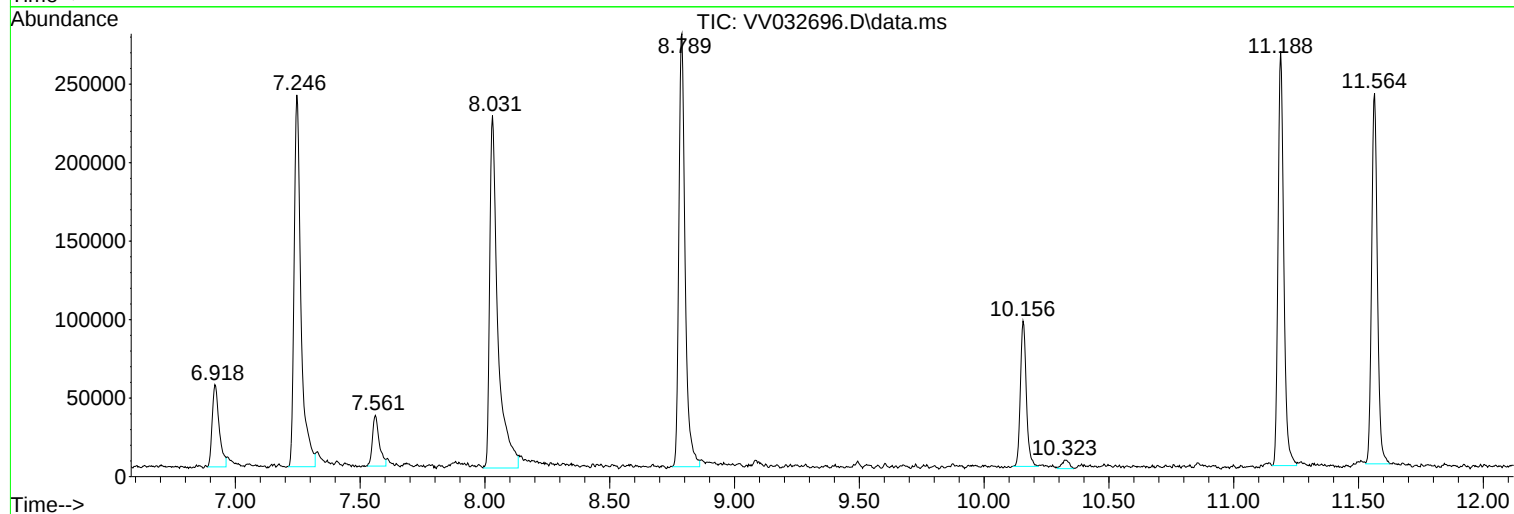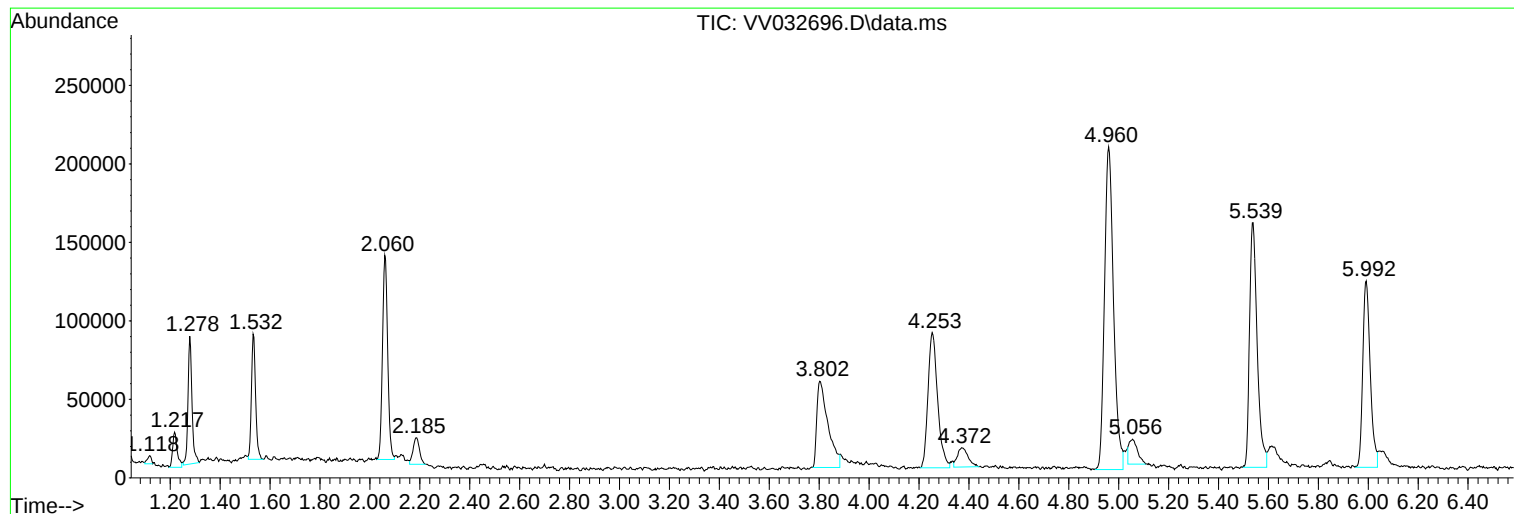

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032696.D
Acq On : 27 Oct 2023 20:09
Operator : SY/MD
Sample : 05055-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4939

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032696.D
Acq On : 27 Oct 2023 20:09
Operator : SY/MD
Sample : 05055-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4939

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc