

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032697.D
 Acq On : 27 Oct 2023 20:34
 Operator : SY/MD
 Sample : 05055-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4987

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	19	25	32	rVB	6851	10278	1.96%	0.223%
2	1.217	49	55	64	rBV	13827	17756	3.39%	0.385%
3	1.278	68	74	86	rVV	82073	89530	17.08%	1.941%
4	1.532	147	153	167	rVB	76857	89324	17.04%	1.937%
5	2.060	308	317	331	rBV	130624	191236	36.49%	4.146%
6	2.185	346	356	369	rVB	18274	37753	7.20%	0.819%
7	3.802	850	859	881	rBV	50179	153439	29.28%	3.327%
8	4.252	978	999	1022	rBV2	89147	243363	46.44%	5.276%
9	4.378	1026	1038	1055	rVB4	11091	34863	6.65%	0.756%
10	4.963	1202	1220	1239	rBV2	203145	524077	100.00%	11.362%
11	5.053	1239	1248	1267	rVB6	18071	53610	10.23%	1.162%
12	5.539	1387	1399	1416	rBV	160805	341505	65.16%	7.404%
13	5.612	1418	1422	1439	rVB4	11885	28377	5.41%	0.615%
14	5.992	1526	1540	1554	rBV2	120656	252051	48.09%	5.465%
15	6.918	1819	1828	1840	rBV2	54655	102882	19.63%	2.231%
16	7.246	1920	1930	1952	rBV	234838	458526	87.49%	9.941%
17	7.561	2018	2028	2038	rBV3	30259	57358	10.94%	1.244%
18	8.030	2165	2174	2206	rBV	219771	486385	92.81%	10.545%
19	8.789	2398	2410	2435	rBV	265538	480271	91.64%	10.412%
20	10.156	2824	2835	2847	rBV	94767	155733	29.72%	3.376%
21	10.329	2881	2889	2894	rVB	4818	5533	1.06%	0.120%
22	11.188	3146	3156	3178	rBV	263084	421865	80.50%	9.146%
23	11.564	3262	3273	3289	rVB	233299	376739	71.89%	8.168%




Sum of corrected areas: 4612454

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032697.D
Acq On : 27 Oct 2023 20:34
Operator : SY/MD
Sample : 05055-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4987

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

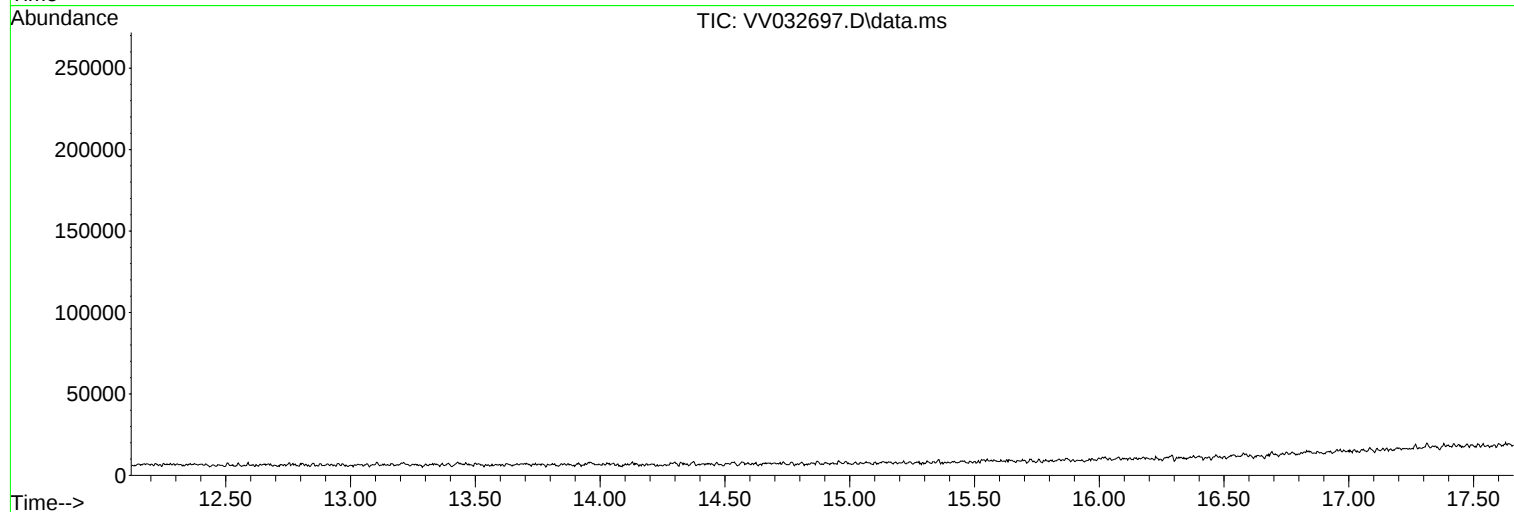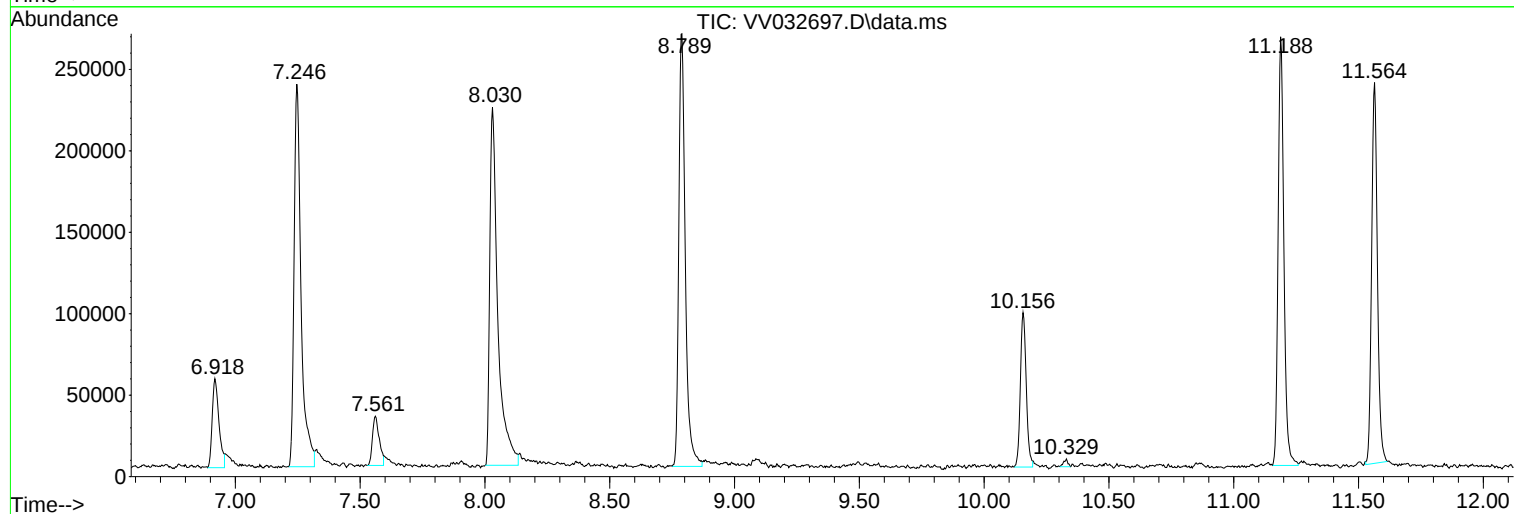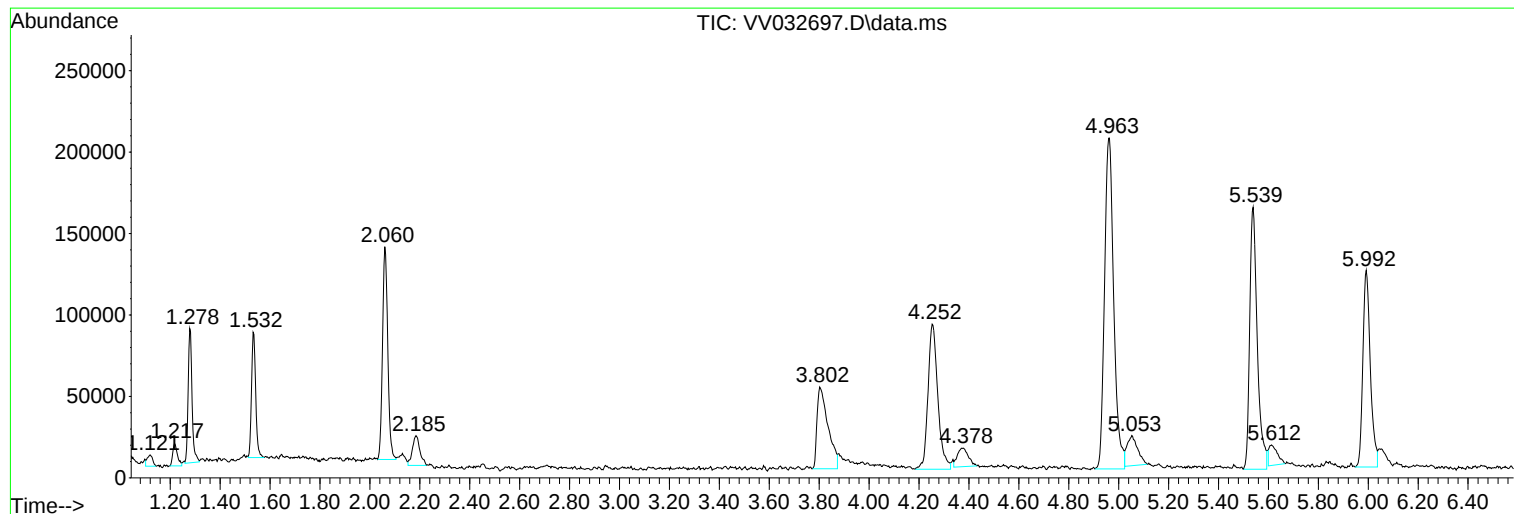

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032697.D
Acq On : 27 Oct 2023 20:34
Operator : SY/MD
Sample : 05055-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4987

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032697.D
Acq On : 27 Oct 2023 20:34
Operator : SY/MD
Sample : 05055-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4987

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc