

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032698.D
 Acq On : 27 Oct 2023 20:58
 Operator : SY/MD
 Sample : 05055-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4991

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	34	rVB	7992	9868	1.94%	0.217%
2	1.217	47	55	62	rBV	15383	19219	3.78%	0.422%
3	1.278	66	74	86	rVV	83947	93561	18.42%	2.056%
4	1.532	146	153	161	rBV	75997	89718	17.67%	1.971%
5	2.060	307	317	330	rBV	135295	196723	38.74%	4.323%
6	2.185	349	356	368	rVB2	18689	34847	6.86%	0.766%
7	3.809	852	861	892	rBV	51085	172398	33.95%	3.788%
8	4.252	985	999	1017	rBV2	84159	218060	42.94%	4.791%
9	4.371	1029	1036	1049	rVB4	11342	25423	5.01%	0.559%
10	4.960	1205	1219	1237	rBV3	203932	507801	100.00%	11.158%
11	5.056	1242	1249	1259	rVB3	11812	26896	5.30%	0.591%
12	5.539	1384	1399	1417	rBV	152943	331530	65.29%	7.285%
13	5.619	1417	1424	1433	rVB7	9662	21262	4.19%	0.467%
14	5.992	1527	1540	1557	rBV2	118718	254696	50.16%	5.596%
15	6.918	1816	1828	1847	rBV	51096	106587	20.99%	2.342%
16	7.246	1919	1930	1952	rBV	233805	448823	88.39%	9.862%
17	7.561	2020	2028	2040	rBV	30626	55639	10.96%	1.223%
18	8.030	2164	2174	2207	rBV	230776	500023	98.47%	10.987%
19	8.789	2397	2410	2430	rBV	265027	473597	93.26%	10.406%
20	9.082	2493	2501	2510	rBV	4826	8835	1.74%	0.194%
21	10.156	2825	2835	2856	rVB	93459	155486	30.62%	3.417%
22	11.188	3145	3156	3174	rBV	255212	415871	81.90%	9.138%
23	11.564	3263	3273	3295	rVB	239669	384132	75.65%	8.441%




Sum of corrected areas: 4550995

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032698.D
Acq On : 27 Oct 2023 20:58
Operator : SY/MD
Sample : 05055-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4991

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

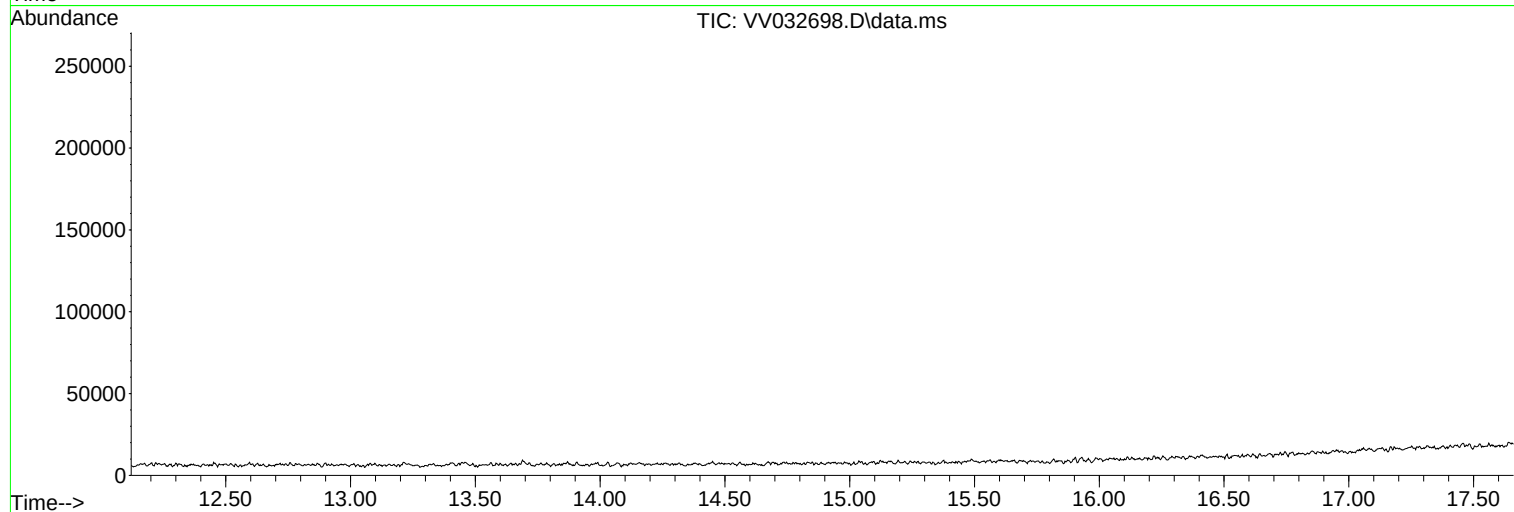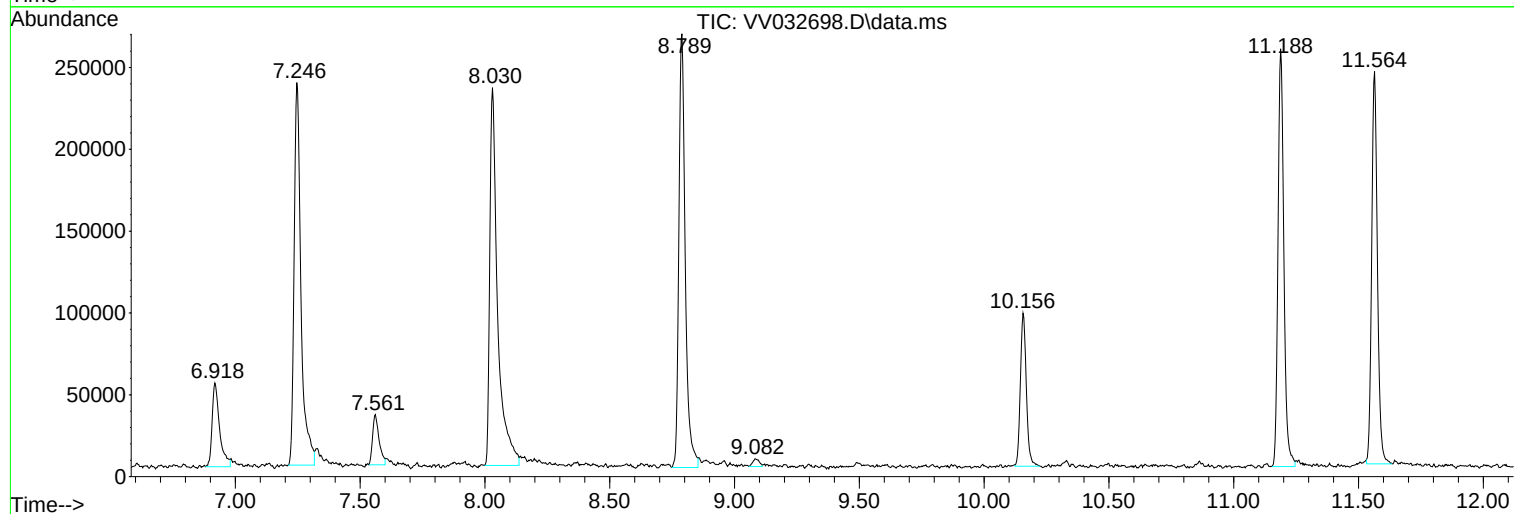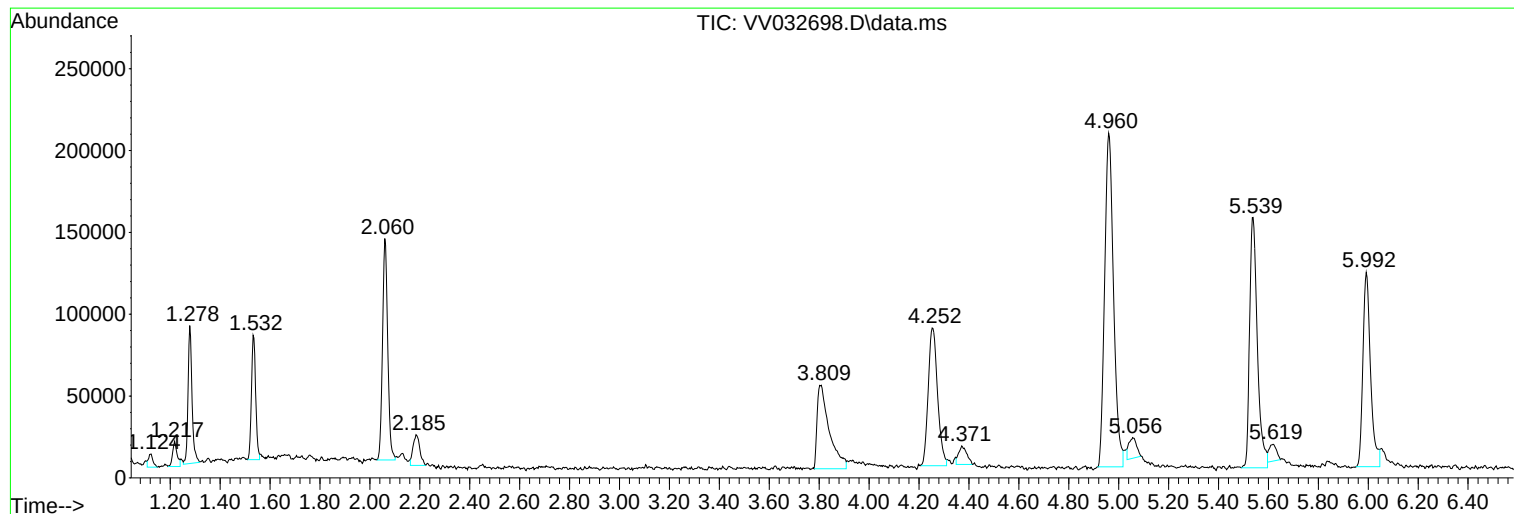

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032698.D
Acq On : 27 Oct 2023 20:58
Operator : SY/MD
Sample : 05055-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4991

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032698.D
Acq On : 27 Oct 2023 20:58
Operator : SY/MD
Sample : 05055-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4991

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc