

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032699.D
 Acq On : 27 Oct 2023 21:22
 Operator : SY/MD
 Sample : 05055-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49F8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	17	25	33	rVB2	6579	11443	2.26%	0.258%
2	1.278	68	74	86	rBV	80576	84327	16.63%	1.904%
3	1.532	147	153	166	rVB	75932	90146	17.77%	2.035%
4	2.060	308	317	330	rBV	126380	184221	36.32%	4.159%
5	2.185	348	356	369	rVB2	17017	32475	6.40%	0.733%
6	3.802	851	859	882	rBV	50007	151426	29.85%	3.419%
7	4.252	981	999	1021	rBV	84446	223546	44.07%	5.047%
8	4.371	1026	1036	1049	rVB4	11816	27192	5.36%	0.614%
9	4.960	1200	1219	1237	rBV3	199976	507224	100.00%	11.452%
10	5.050	1242	1247	1259	rVB7	10915	24590	4.85%	0.555%
11	5.539	1387	1399	1416	rBV	150842	318730	62.84%	7.197%
12	5.992	1525	1540	1554	rBV	115205	246543	48.61%	5.567%
13	6.918	1820	1828	1848	rBV	49812	101285	19.97%	2.287%
14	7.246	1917	1930	1950	rBV	225677	437127	86.18%	9.870%
15	7.561	2016	2028	2037	rBV3	30138	56857	11.21%	1.284%
16	8.030	2164	2174	2209	rBV	219900	491988	97.00%	11.108%
17	8.374	2276	2281	2289	rVB	3878	5826	1.15%	0.132%
18	8.789	2400	2410	2430	rBV	256568	453275	89.36%	10.234%
19	10.156	2824	2835	2851	rBV2	92599	154427	30.45%	3.487%
20	11.188	3145	3156	3177	rBV	252643	410608	80.95%	9.271%
21	11.493	3241	3251	3263	rBV5	16867	38092	7.51%	0.860%
22	11.564	3263	3273	3290	rVB	237392	377594	74.44%	8.526%




Sum of corrected areas: 4428942

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032699.D
Acq On : 27 Oct 2023 21:22
Operator : SY/MD
Sample : 05055-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

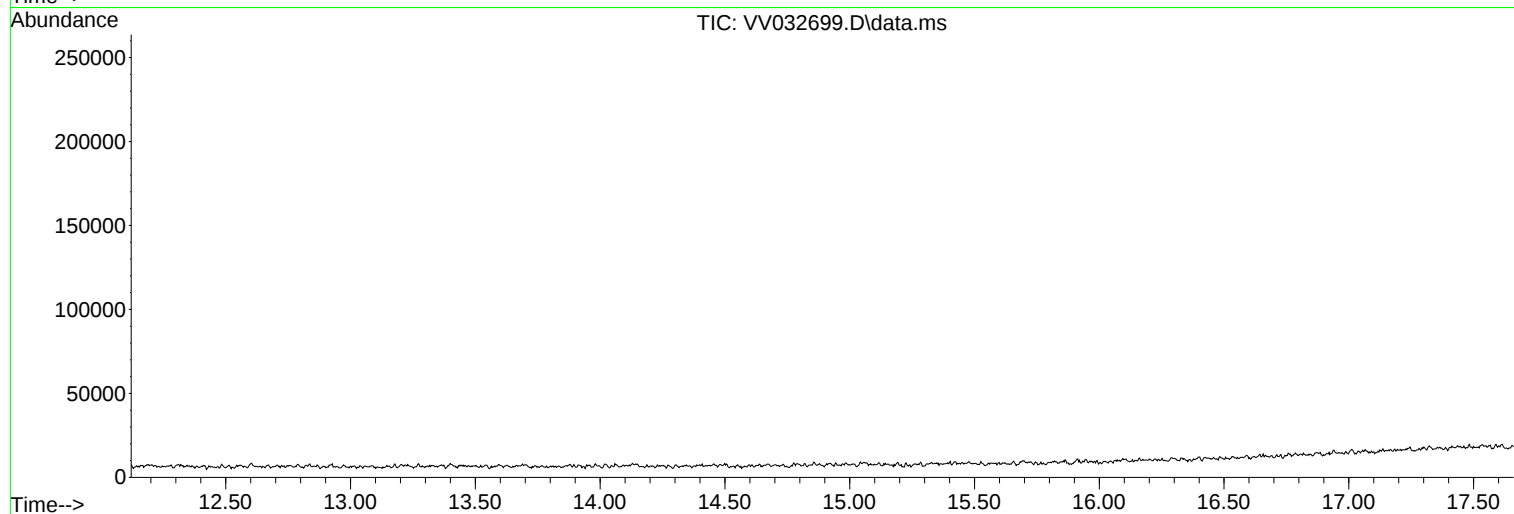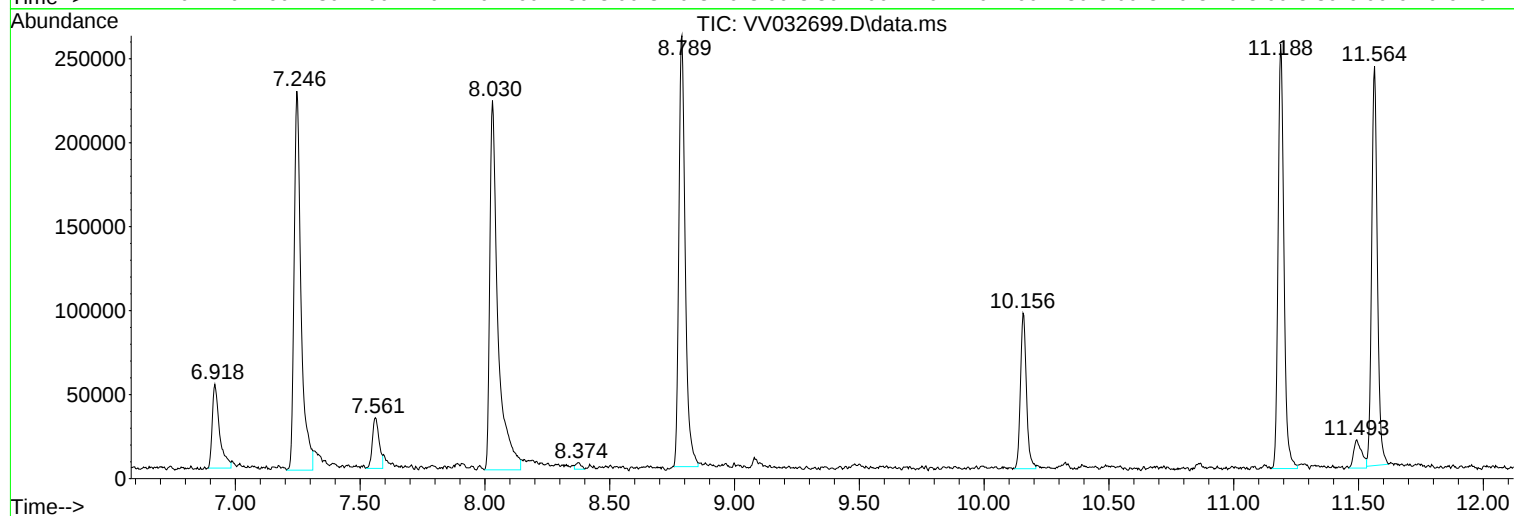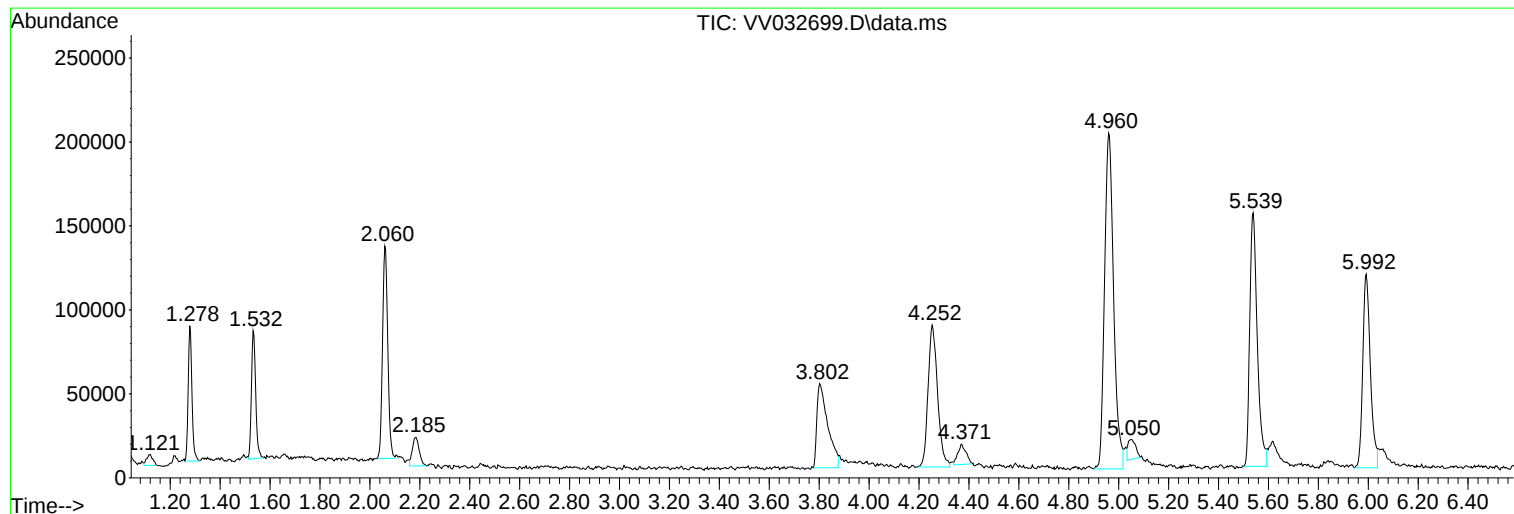

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032699.D
Acq On : 27 Oct 2023 21:22
Operator : SY/MD
Sample : 05055-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032699.D
Acq On : 27 Oct 2023 21:22
Operator : SY/MD
Sample : 05055-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49F8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc