

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032702.D
 Acq On : 27 Oct 2023 22:35
 Operator : SY/MD
 Sample : 05055-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49G7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	61	rBV	13955	15962	2.65%	0.347%
2	1.278	67	74	87	rBV	73919	80165	13.33%	1.741%
3	1.532	146	153	164	rBV	68229	79060	13.14%	1.717%
4	2.060	308	317	329	rBV	117732	170224	28.30%	3.696%
5	2.185	347	356	365	rVB	15553	27922	4.64%	0.606%
6	3.812	850	862	881	rBV3	48395	158504	26.35%	3.442%
7	4.252	986	999	1020	rBV	73911	195818	32.55%	4.252%
8	4.368	1026	1035	1048	rVB3	8950	21160	3.52%	0.459%
9	4.960	1202	1219	1238	rBV3	184738	475498	79.05%	10.325%
10	5.535	1388	1398	1415	rBV	192072	398232	66.20%	8.647%
11	5.992	1527	1540	1554	rBV2	108053	225848	37.54%	4.904%
12	6.918	1815	1828	1842	rBV3	47069	94921	15.78%	2.061%
13	7.246	1919	1930	1949	rBV	212515	408133	67.85%	8.862%
14	7.561	2018	2028	2042	rBV2	27195	52822	8.78%	1.147%
15	8.030	2165	2174	2207	rBV	206123	466144	77.49%	10.122%
16	8.789	2395	2410	2434	rBV	334385	601548	100.00%	13.062%
17	9.082	2493	2501	2511	rBV	6007	12466	2.07%	0.271%
18	9.487	2618	2627	2631	rBV	4417	7485	1.24%	0.163%
19	9.892	2745	2753	2758	rBV10	4937	7465	1.24%	0.162%
20	10.156	2825	2835	2850	rVB	87461	142074	23.62%	3.085%
21	11.188	3145	3156	3178	rVV	330918	518769	86.24%	11.265%
22	11.294	3182	3189	3202	rVB	6867	13779	2.29%	0.299%
23	11.493	3240	3251	3262	rBV6	14489	32544	5.41%	0.707%
24	11.564	3262	3273	3290	rVB	224134	362177	60.21%	7.865%
25	11.953	3386	3394	3405	rBV	7274	10993	1.83%	0.239%
26	14.355	4130	4141	4151	rBV	14516	25491	4.24%	0.554%




Sum of corrected areas: 4605204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032702.D
Acq On : 27 Oct 2023 22:35
Operator : SY/MD
Sample : 05055-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

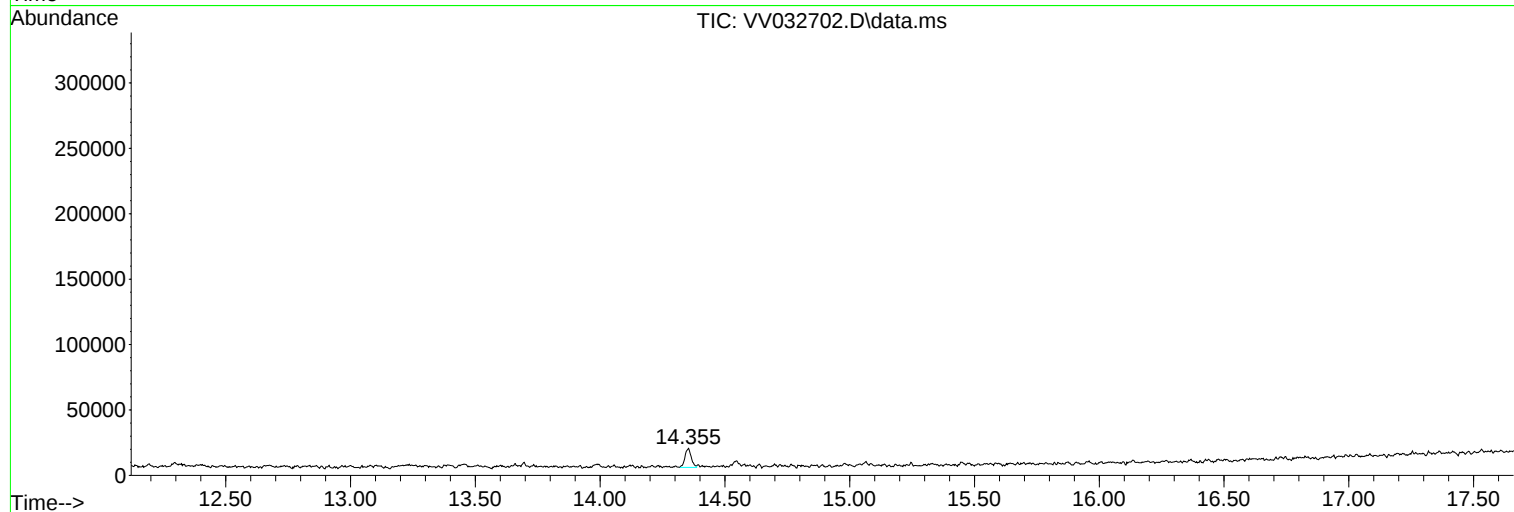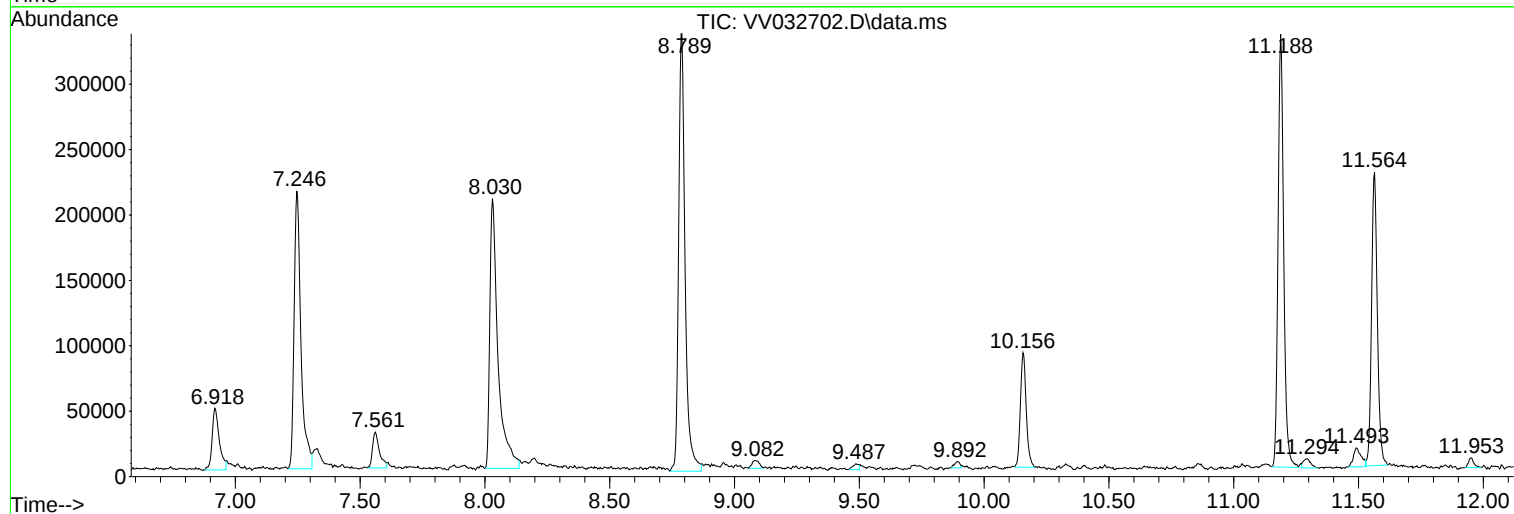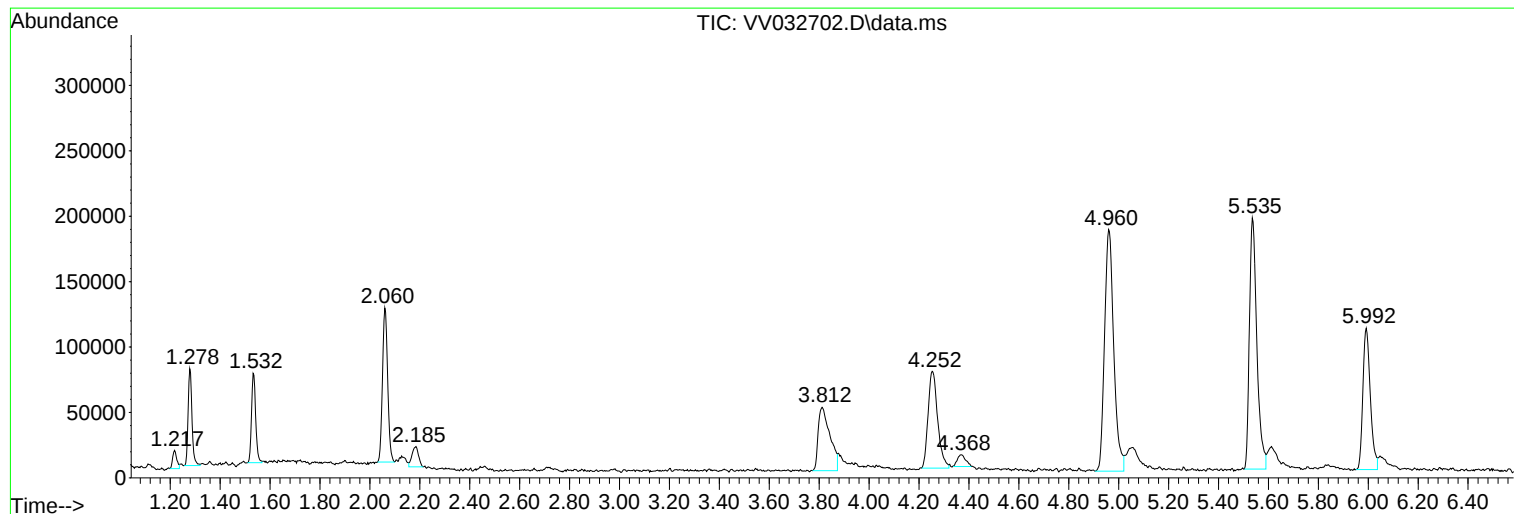

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032702.D
Acq On : 27 Oct 2023 22:35
Operator : SY/MD
Sample : 05055-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032702.D
Acq On : 27 Oct 2023 22:35
Operator : SY/MD
Sample : 05055-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc