

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032712.D
 Acq On : 28 Oct 2023 03:02
 Operator : SY/MD
 Sample : 05055-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A48Z7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	16	23	32	rVB2	7696	11182	2.24%	0.255%
2	1.217	49	55	61	rBV	7157	9214	1.85%	0.210%
3	1.278	66	74	83	rVV	78520	85448	17.13%	1.949%
4	1.532	146	153	168	rBV	74406	88360	17.71%	2.015%
5	2.060	305	317	330	rBV	125125	186841	37.46%	4.261%
6	2.182	347	355	368	rVB3	16694	29697	5.95%	0.677%
7	3.806	850	860	887	rBV	48568	156690	31.41%	3.574%
8	4.253	984	999	1021	rBV2	82737	219684	44.04%	5.011%
9	4.368	1026	1035	1039	rBV4	8541	14058	2.82%	0.321%
10	4.960	1204	1219	1237	rBV2	194190	498787	100.00%	11.376%
11	5.050	1243	1247	1257	rVB4	10607	17664	3.54%	0.403%
12	5.539	1388	1399	1417	rBV2	147330	315044	63.16%	7.185%
13	5.992	1528	1540	1555	rBV2	114279	241293	48.38%	5.503%
14	6.918	1818	1828	1847	rBV3	48399	100445	20.14%	2.291%
15	7.246	1918	1930	1949	rBV	227642	427920	85.79%	9.760%
16	7.561	2017	2028	2045	rBV2	27851	63460	12.72%	1.447%
17	8.031	2163	2174	2200	rBV	215824	476560	95.54%	10.869%
18	8.789	2398	2410	2431	rBV	257897	460099	92.24%	10.494%
19	8.957	2455	2462	2467	rBV7	5008	6945	1.39%	0.158%
20	9.082	2493	2501	2512	rBV6	7731	13336	2.67%	0.304%
21	9.490	2618	2628	2638	rBV6	5259	10009	2.01%	0.228%
22	10.156	2824	2835	2848	rBV	92003	149459	29.96%	3.409%
23	10.323	2884	2887	2896	rVB7	5519	7226	1.45%	0.165%
24	10.857	3044	3053	3064	rBV7	5333	11001	2.21%	0.251%
25	11.188	3144	3156	3176	rVV	250637	405040	81.21%	9.238%
26	11.493	3244	3251	3254	rBV8	7805	9486	1.90%	0.216%
27	11.564	3260	3273	3289	rVB	232080	369505	74.08%	8.428%




Sum of corrected areas: 4384453

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032712.D
Acq On : 28 Oct 2023 03:02
Operator : SY/MD
Sample : 05055-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

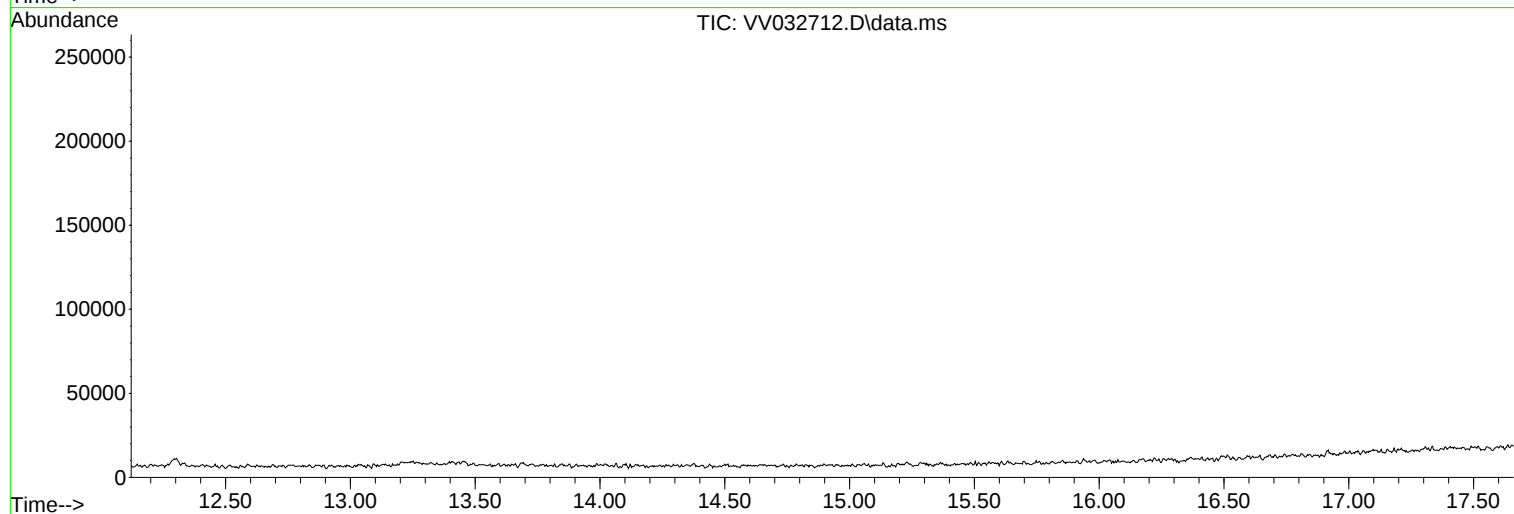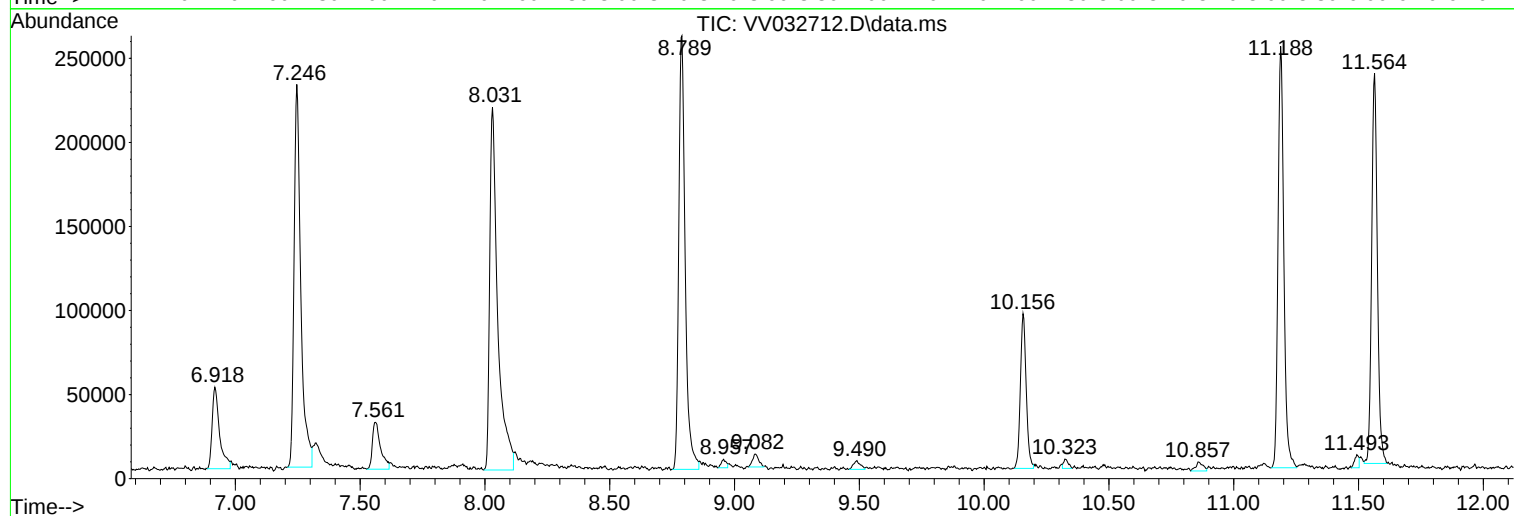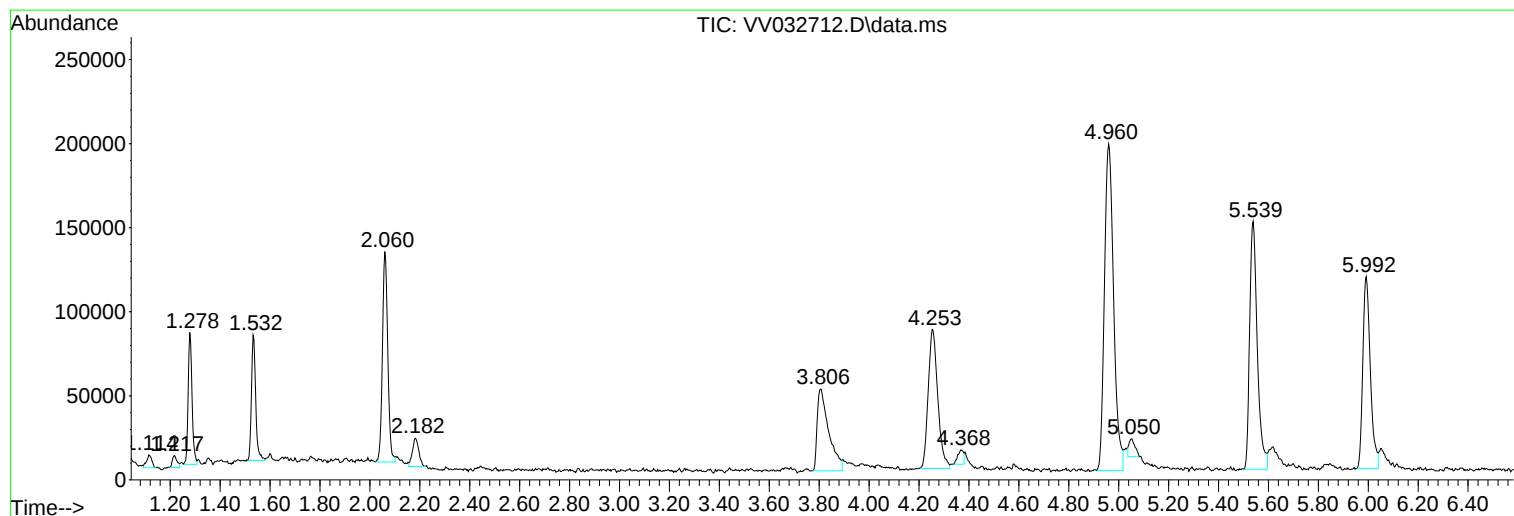

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032712.D
Acq On : 28 Oct 2023 03:02
Operator : SY/MD
Sample : 05055-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032712.D
Acq On : 28 Oct 2023 03:02
Operator : SY/MD
Sample : 05055-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A48Z7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc