

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032713.D
 Acq On : 28 Oct 2023 03:26
 Operator : SY/MD
 Sample : 05055-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4972

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	18	24	30	rVB	7922	9838	1.97%	0.222%
2	1.217	49	55	60	rBV	9742	11404	2.29%	0.257%
3	1.278	66	74	82	rBV	78374	85196	17.08%	1.918%
4	1.532	147	153	163	rBV	73174	86014	17.24%	1.937%
5	2.060	306	317	333	rBV	124226	186422	37.37%	4.198%
6	2.182	349	355	368	rVB2	17218	32056	6.43%	0.722%
7	3.806	850	860	887	rBV3	55190	186717	37.43%	4.204%
8	4.256	984	1000	1021	rBV2	83649	217981	43.70%	4.908%
9	4.368	1022	1035	1049	rVB2	10118	25900	5.19%	0.583%
10	4.960	1205	1219	1238	rBV3	196577	493543	98.94%	11.113%
11	5.053	1241	1248	1261	rVB4	13318	33847	6.79%	0.762%
12	5.539	1387	1399	1414	rBV	147524	319238	64.00%	7.188%
13	5.992	1526	1540	1558	rBV	114552	249199	49.96%	5.611%
14	6.918	1816	1828	1842	rBV2	48693	101331	20.31%	2.282%
15	7.246	1919	1930	1952	rBV	225962	442524	88.71%	9.965%
16	7.561	2021	2028	2040	rBV2	27608	49249	9.87%	1.109%
17	8.031	2161	2174	2211	rBV	218429	498827	100.00%	11.232%
18	8.789	2397	2410	2435	rBV	261218	471442	94.51%	10.616%
19	10.156	2825	2835	2853	rVB	91332	154218	30.92%	3.473%
20	11.188	3146	3156	3177	rBV	256510	408414	81.87%	9.196%
21	11.500	3245	3253	3255	rBV9	5230	5898	1.18%	0.133%
22	11.564	3261	3273	3295	rVB	228541	371733	74.52%	8.370%




Sum of corrected areas: 4440991

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032713.D
Acq On : 28 Oct 2023 03:26
Operator : SY/MD
Sample : 05055-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4972

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

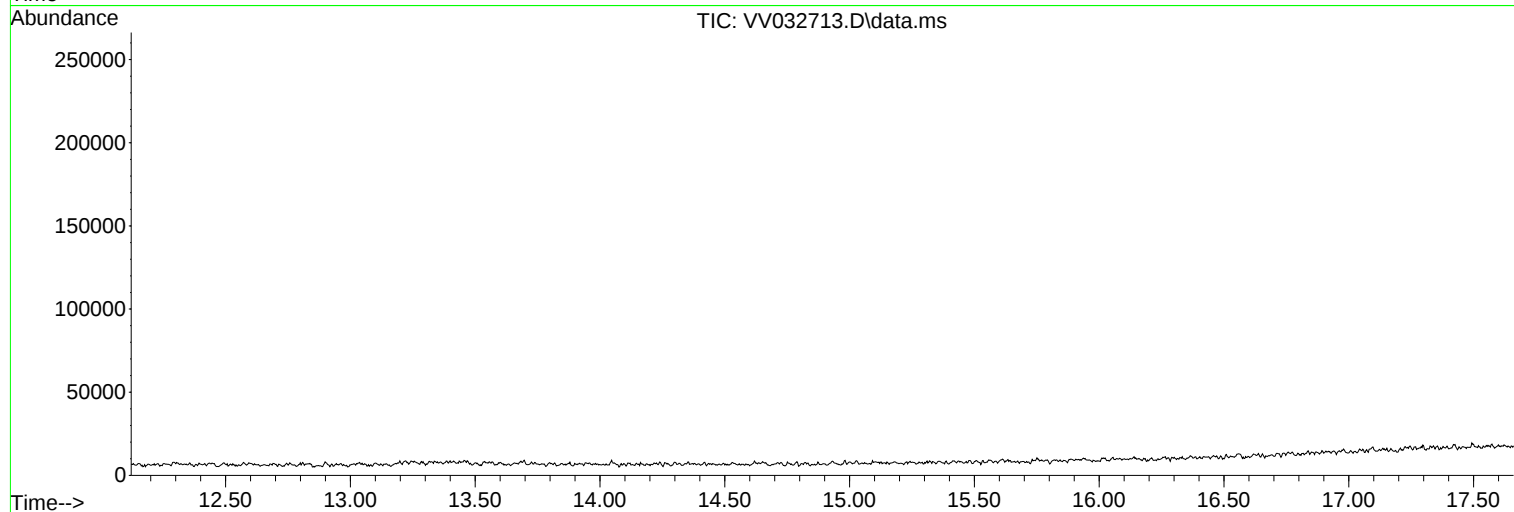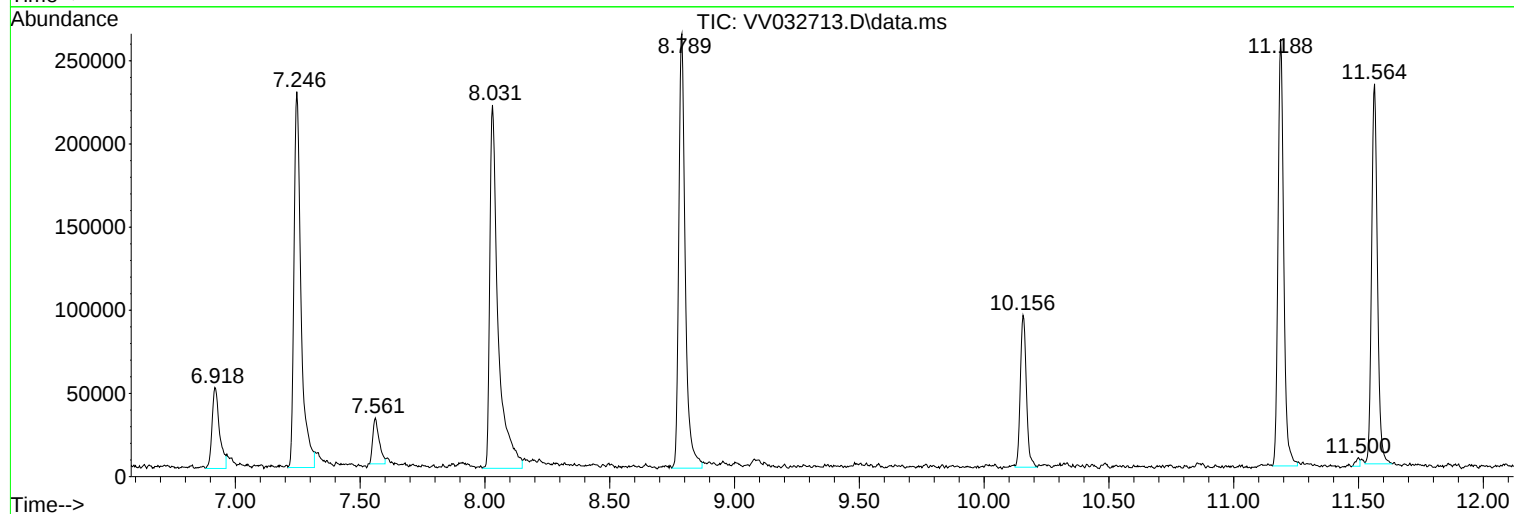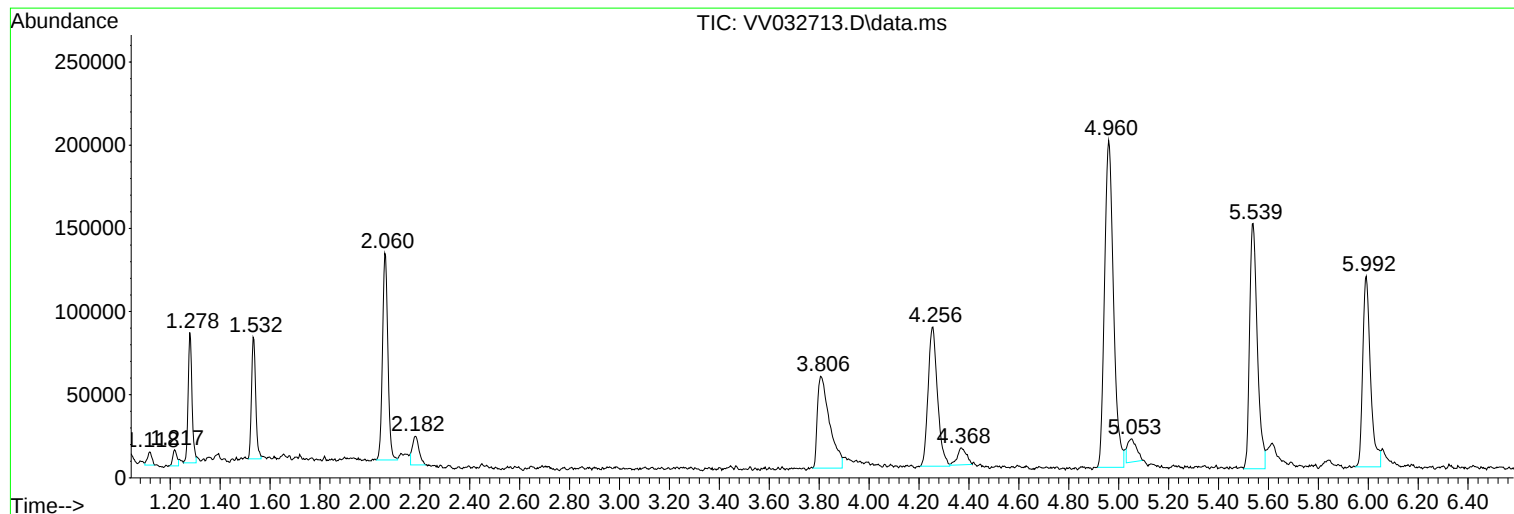

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032713.D
Acq On : 28 Oct 2023 03:26
Operator : SY/MD
Sample : 05055-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4972

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032713.D
Acq On : 28 Oct 2023 03:26
Operator : SY/MD
Sample : 05055-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4972

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
