

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032717.D
 Acq On : 28 Oct 2023 05:03
 Operator : SY/MD
 Sample : 05019-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49B9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	16	23	32	rVB2	9186	14326	3.08%	0.344%
2	1.278	67	74	85	rBV	72219	75394	16.23%	1.810%
3	1.532	146	153	165	rBV	68985	80704	17.37%	1.938%
4	2.060	307	317	332	rBV	123279	180066	38.76%	4.324%
5	2.130	337	339	346	rVV8	4811	5869	1.26%	0.141%
6	2.179	346	354	370	rVB3	15011	31317	6.74%	0.752%
7	3.806	852	860	888	rBV2	43033	146448	31.53%	3.516%
8	4.256	983	1000	1022	rBV	80717	216332	46.57%	5.194%
9	4.368	1022	1035	1041	rBV4	7474	15346	3.30%	0.368%
10	4.960	1204	1219	1237	rBV3	182334	464528	100.00%	11.154%
11	5.053	1243	1248	1267	rVB7	14355	31464	6.77%	0.755%
12	5.539	1387	1399	1417	rBV2	145468	315794	67.98%	7.583%
13	5.992	1528	1540	1556	rBV2	108632	232005	49.94%	5.571%
14	6.918	1819	1828	1848	rBV3	43921	91690	19.74%	2.202%
15	7.246	1919	1930	1953	rBV	212577	407258	87.67%	9.779%
16	7.561	2020	2028	2041	rBV2	26892	49099	10.57%	1.179%
17	8.031	2164	2174	2210	rBV	196478	447634	96.36%	10.748%
18	8.789	2400	2410	2427	rBV	252448	443701	95.52%	10.654%
19	10.156	2826	2835	2850	rBV2	83983	139101	29.94%	3.340%
20	11.188	3143	3156	3172	rBV	246568	392188	84.43%	9.417%
21	11.493	3242	3251	3262	rBV4	16883	34683	7.47%	0.833%
22	11.564	3262	3273	3288	rVB	218167	349714	75.28%	8.397%




Sum of corrected areas: 4164661

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032717.D
Acq On : 28 Oct 2023 05:03
Operator : SY/MD
Sample : 05019-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49B9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

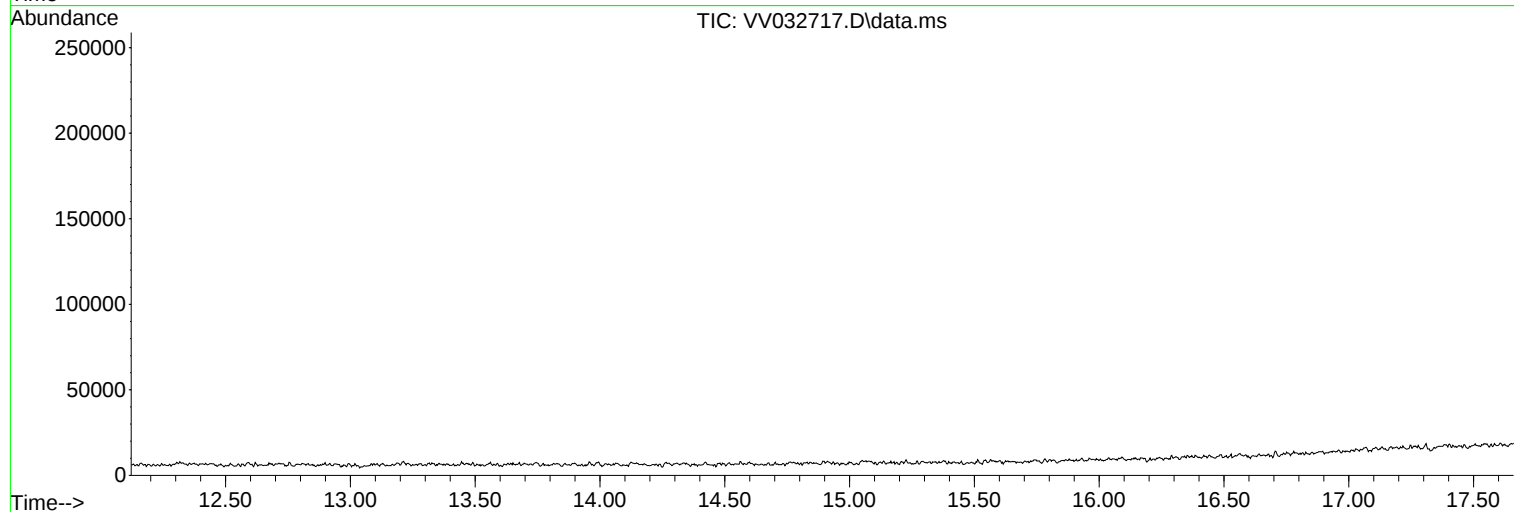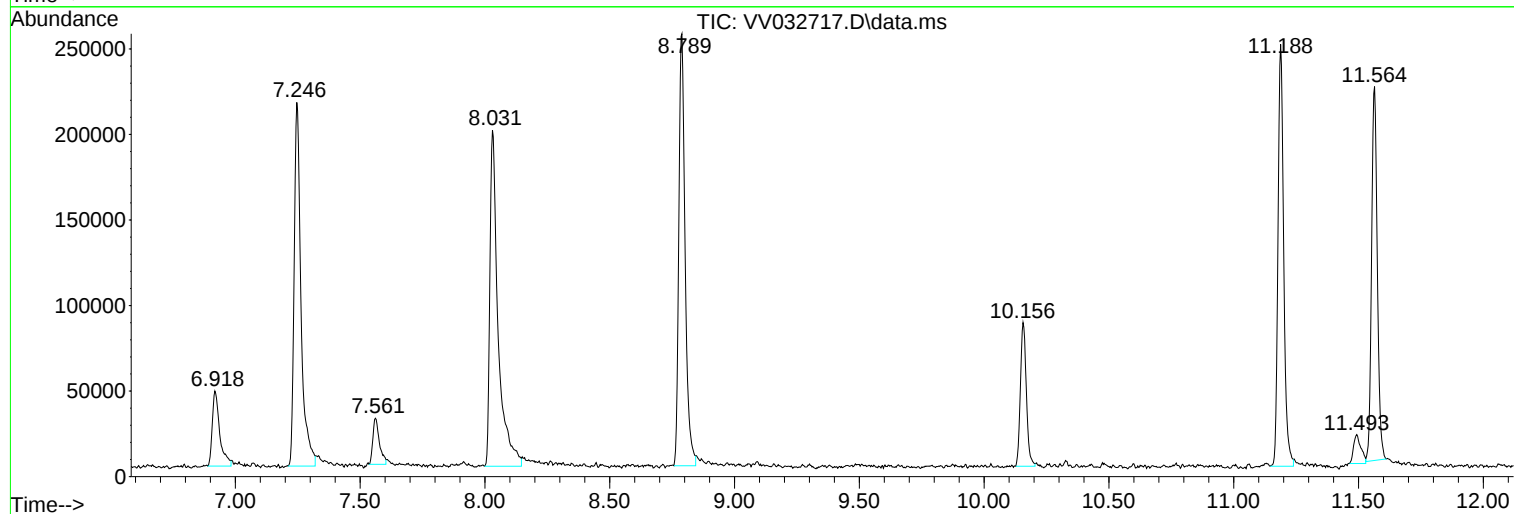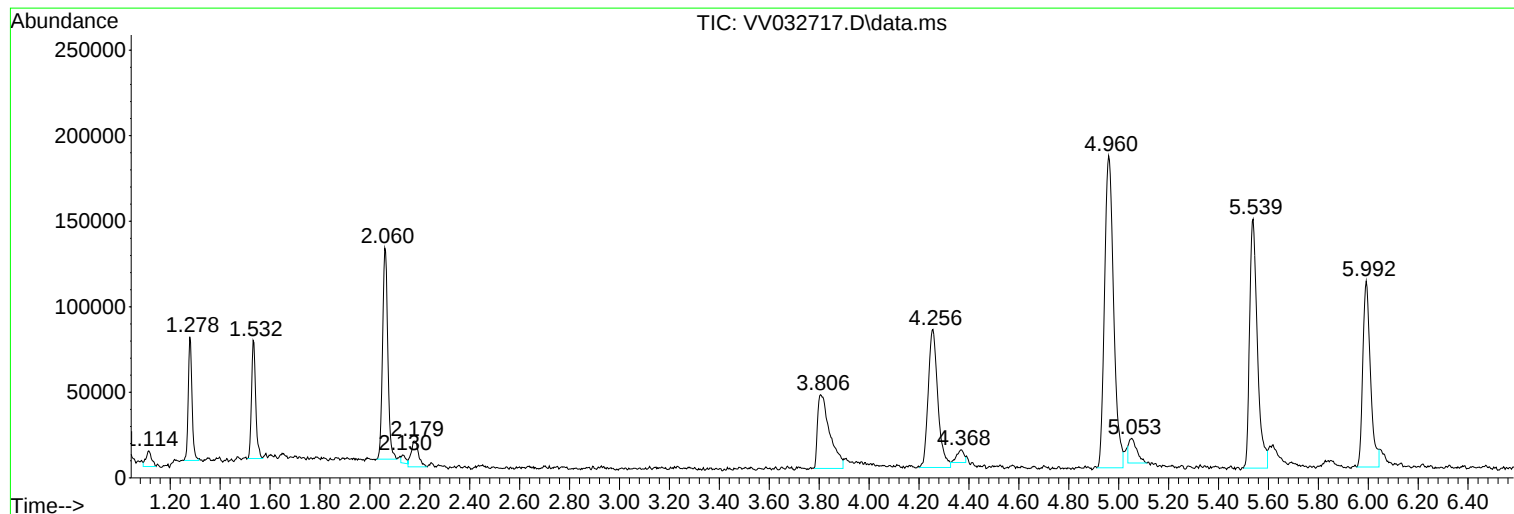

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032717.D
Acq On : 28 Oct 2023 05:03
Operator : SY/MD
Sample : 05019-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49B9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032717.D
Acq On : 28 Oct 2023 05:03
Operator : SY/MD
Sample : 05019-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49B9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc