

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032720.D
 Acq On : 28 Oct 2023 06:16
 Operator : SY/MD
 Sample : 05019-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4992

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.118	19	24	32	rVB	6926	8514	1.72%	0.197%
2	1.217	49	55	60	rBV	8707	11055	2.23%	0.255%
3	1.278	68	74	86	rBV	75529	80122	16.19%	1.850%
4	1.532	146	153	164	rBV	71639	86373	17.45%	1.994%
5	2.060	307	317	332	rBV	122681	182780	36.93%	4.219%
6	2.182	348	355	365	rVB2	18131	32808	6.63%	0.757%
7	3.802	851	859	888	rBV2	52241	171560	34.66%	3.960%
8	4.253	982	999	1020	rBV2	81758	213661	43.17%	4.932%
9	4.372	1025	1036	1053	rVB3	11376	32133	6.49%	0.742%
10	4.960	1201	1219	1240	rBV4	190397	494974	100.00%	11.426%
11	5.535	1388	1398	1416	rBV	154781	326203	65.90%	7.530%
12	5.992	1529	1540	1557	rBV	113529	239997	48.49%	5.540%
13	6.918	1814	1828	1840	rBV2	46968	93188	18.83%	2.151%
14	7.246	1917	1930	1953	rBV	217847	425207	85.90%	9.815%
15	7.561	2018	2028	2041	rBV2	28256	56209	11.36%	1.298%
16	7.908	2130	2136	2144	rVB2	4113	6132	1.24%	0.142%
17	8.031	2165	2174	2210	rBV3	204815	470458	95.05%	10.860%
18	8.789	2398	2410	2431	rBV	265138	478703	96.71%	11.050%
19	10.156	2825	2835	2853	rVB	89123	149802	30.26%	3.458%
20	11.188	3145	3156	3171	rBV	259704	410704	82.97%	9.481%
21	11.564	3261	3273	3287	rBV	222188	361416	73.02%	8.343%




Sum of corrected areas: 4331999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032720.D
Acq On : 28 Oct 2023 06:16
Operator : SY/MD
Sample : 05019-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4992

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

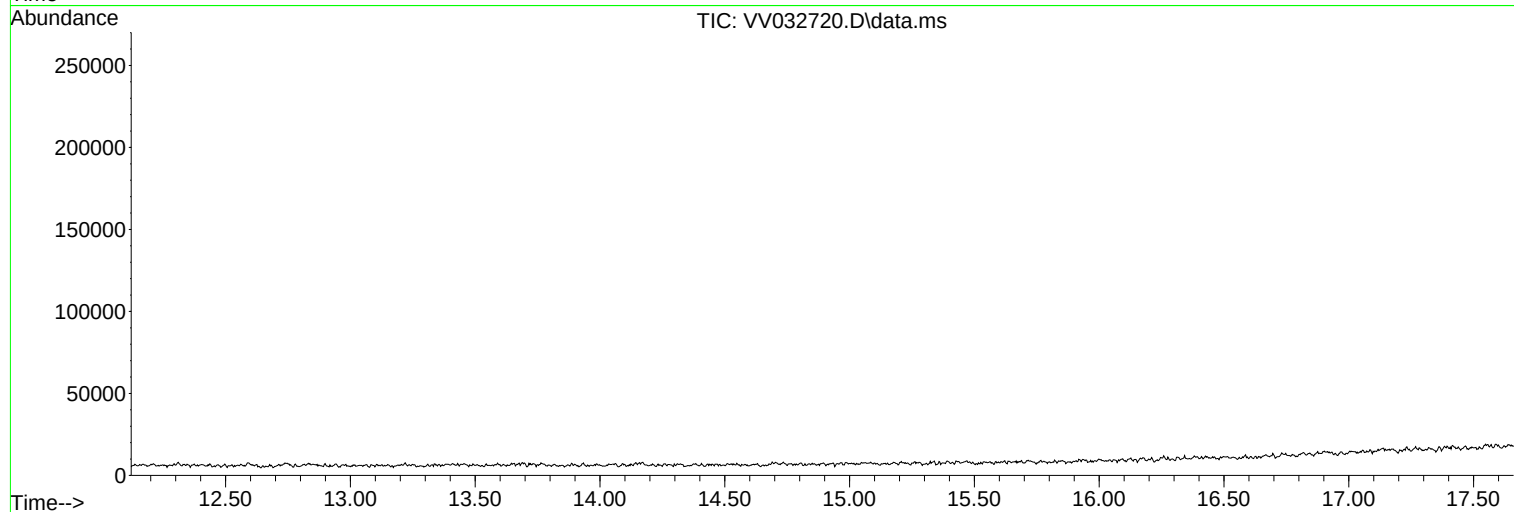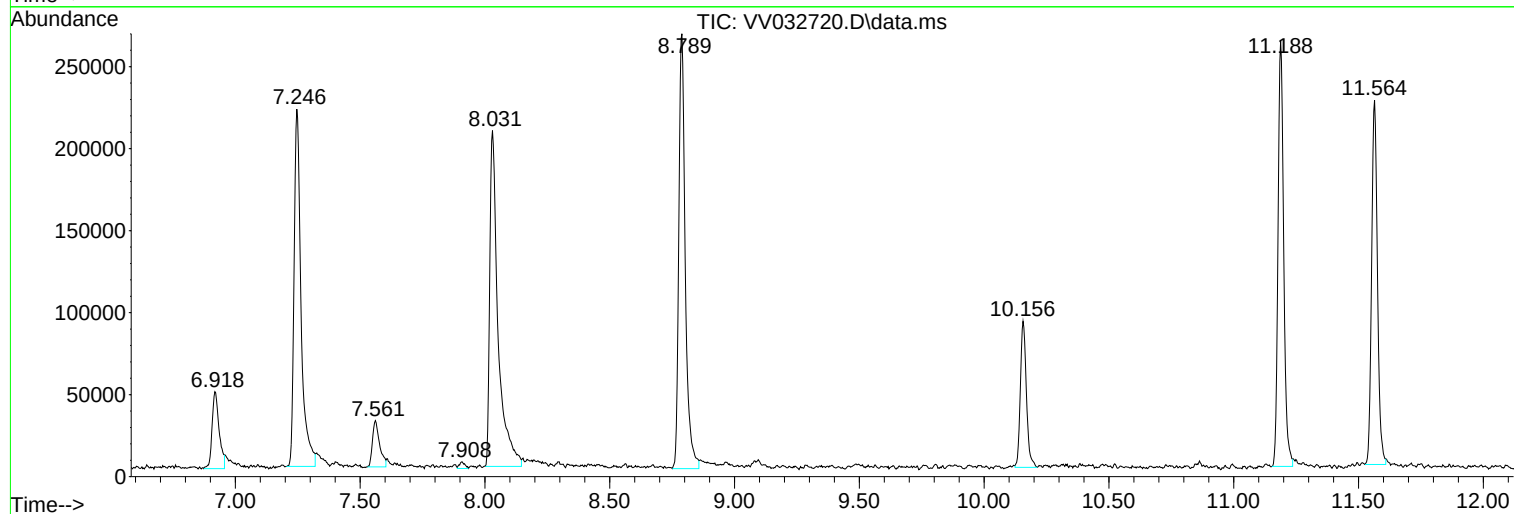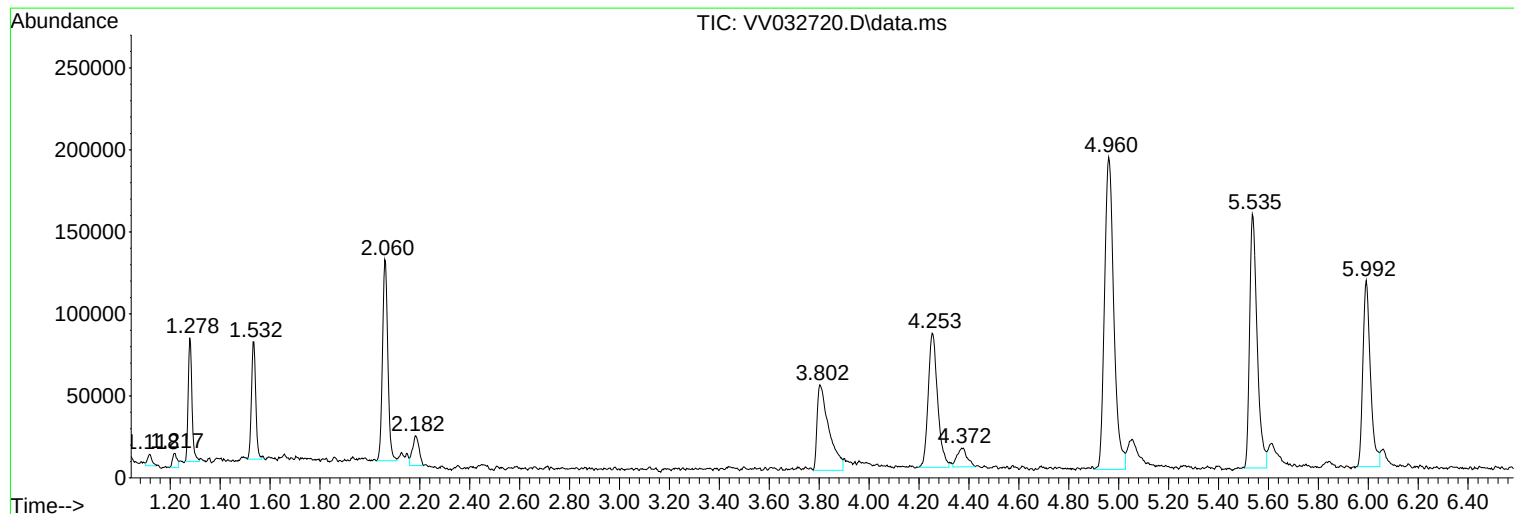

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032720.D
Acq On : 28 Oct 2023 06:16
Operator : SY/MD
Sample : 05019-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4992

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032720.D
Acq On : 28 Oct 2023 06:16
Operator : SY/MD
Sample : 05019-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4992

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc