

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032723.D
 Acq On : 28 Oct 2023 07:29
 Operator : SY/MD
 Sample : 05019-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49B1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	18	24	31	rVB	5678	6655	1.37%	0.151%
2	1.217	46	55	61	rBV	14054	18565	3.83%	0.422%
3	1.278	67	74	84	rBV	75993	81050	16.74%	1.842%
4	1.388	103	108	117	rVB2	4853	6027	1.24%	0.137%
5	1.532	144	153	165	rBV	73032	89593	18.50%	2.036%
6	2.060	308	317	329	rBV	125531	180995	37.38%	4.114%
7	2.124	334	337	348	rVV3	6923	10042	2.07%	0.228%
8	2.182	348	355	368	rVB2	17373	31987	6.61%	0.727%
9	3.805	845	860	885	rBV2	58201	197558	40.80%	4.490%
10	4.252	985	999	1021	rBV	83711	218069	45.03%	4.957%
11	4.368	1026	1035	1040	rBV4	9020	14634	3.02%	0.333%
12	4.960	1205	1219	1238	rBV2	190389	484260	100.00%	11.007%
13	5.050	1244	1247	1258	rVB6	10569	18528	3.83%	0.421%
14	5.539	1387	1399	1415	rBV	150924	319016	65.88%	7.251%
15	5.831	1485	1490	1496	rBV9	3834	5826	1.20%	0.132%
16	5.992	1524	1540	1553	rBV2	113261	240682	49.70%	5.471%
17	6.918	1818	1828	1845	rBV2	46715	93772	19.36%	2.131%
18	7.246	1919	1930	1961	rBV	219024	438197	90.49%	9.960%
19	7.561	2020	2028	2047	rBV3	28698	60828	12.56%	1.383%
20	8.030	2164	2174	2207	rBV2	204739	464466	95.91%	10.557%
21	8.789	2399	2410	2431	rBV	264537	469867	97.03%	10.680%
22	9.082	2493	2501	2513	rBV	6094	12021	2.48%	0.273%
23	10.156	2824	2835	2852	rBV2	90432	152957	31.59%	3.477%
24	10.860	3048	3054	3062	rVB2	3727	5417	1.12%	0.123%
25	11.188	3144	3156	3176	rBV	261141	417875	86.29%	9.498%
26	11.564	3262	3273	3290	rBV	223873	360636	74.47%	8.197%




Sum of corrected areas: 4399523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032723.D
Acq On : 28 Oct 2023 07:29
Operator : SY/MD
Sample : 05019-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

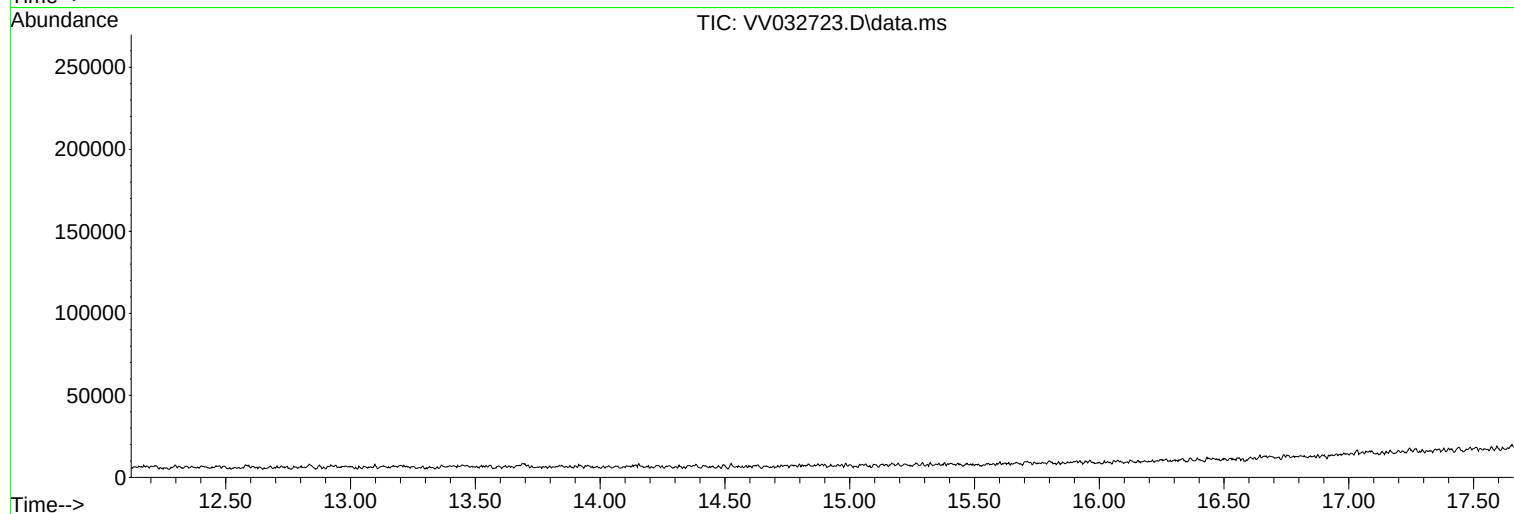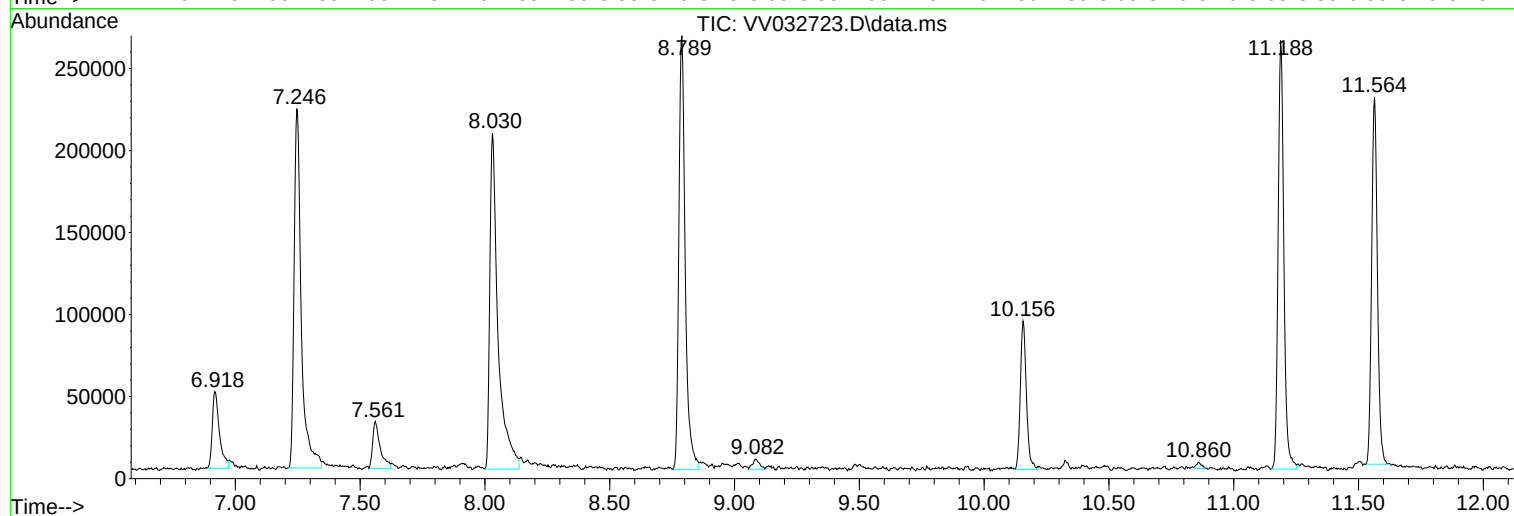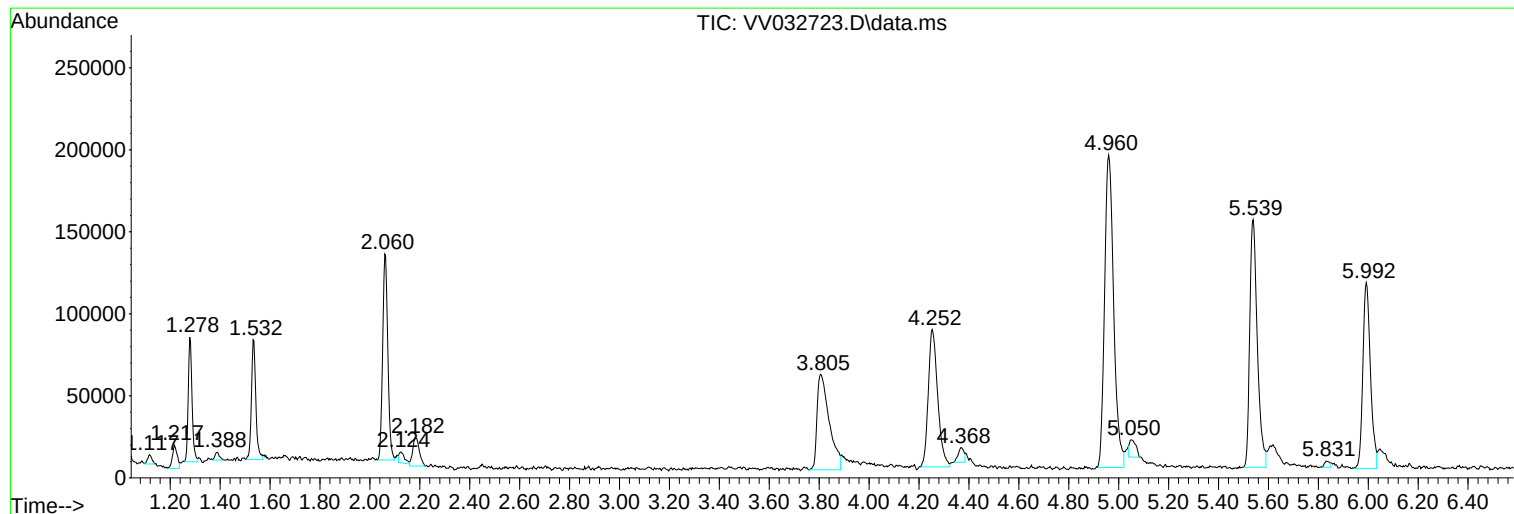

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032723.D
Acq On : 28 Oct 2023 07:29
Operator : SY/MD
Sample : 05019-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032723.D
Acq On : 28 Oct 2023 07:29
Operator : SY/MD
Sample : 05019-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49B1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc