

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032727.D
 Acq On : 28 Oct 2023 09:05
 Operator : SY/MD
 Sample : 05019-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49H2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	33	rVB	7827	11679	2.22%	0.275%
2	1.278	68	74	89	rVB	67410	72254	13.75%	1.698%
3	1.455	116	129	131	rBV	6341	10405	1.98%	0.245%
4	1.532	147	153	168	rVB	65228	77757	14.79%	1.828%
5	2.063	309	318	330	rBV	110208	163601	31.13%	3.846%
6	2.179	348	354	367	rVB4	13043	25124	4.78%	0.591%
7	3.796	849	857	878	rBV	51331	147837	28.13%	3.475%
8	4.256	982	1000	1019	rBV	73838	195143	37.13%	4.587%
9	4.368	1029	1035	1044	rVB7	6159	9888	1.88%	0.232%
10	4.963	1204	1220	1238	rBV3	171903	440360	83.78%	10.351%
11	5.053	1243	1248	1259	rVB5	10408	22318	4.25%	0.525%
12	5.539	1385	1399	1417	rBV	174876	371616	70.70%	8.736%
13	5.992	1525	1540	1559	rBV	105114	229774	43.72%	5.401%
14	6.921	1818	1829	1844	rBV	42953	90419	17.20%	2.125%
15	7.249	1917	1931	1951	rBV	194988	379211	72.15%	8.914%
16	7.561	2020	2028	2039	rBV	25598	48164	9.16%	1.132%
17	8.031	2163	2174	2205	rBV2	208864	472999	89.99%	11.119%
18	8.789	2399	2410	2429	rBV	302463	525603	100.00%	12.355%
19	10.156	2822	2835	2847	rBV	89733	145548	27.69%	3.421%
20	11.188	3144	3156	3174	rBV	295593	470729	89.56%	11.065%
21	11.497	3243	3252	3254	rBV8	6492	6778	1.29%	0.159%
22	11.564	3261	3273	3292	rVB	209293	336876	64.09%	7.919%




Sum of corrected areas: 4254083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032727.D
Acq On : 28 Oct 2023 09:05
Operator : SY/MD
Sample : 05019-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

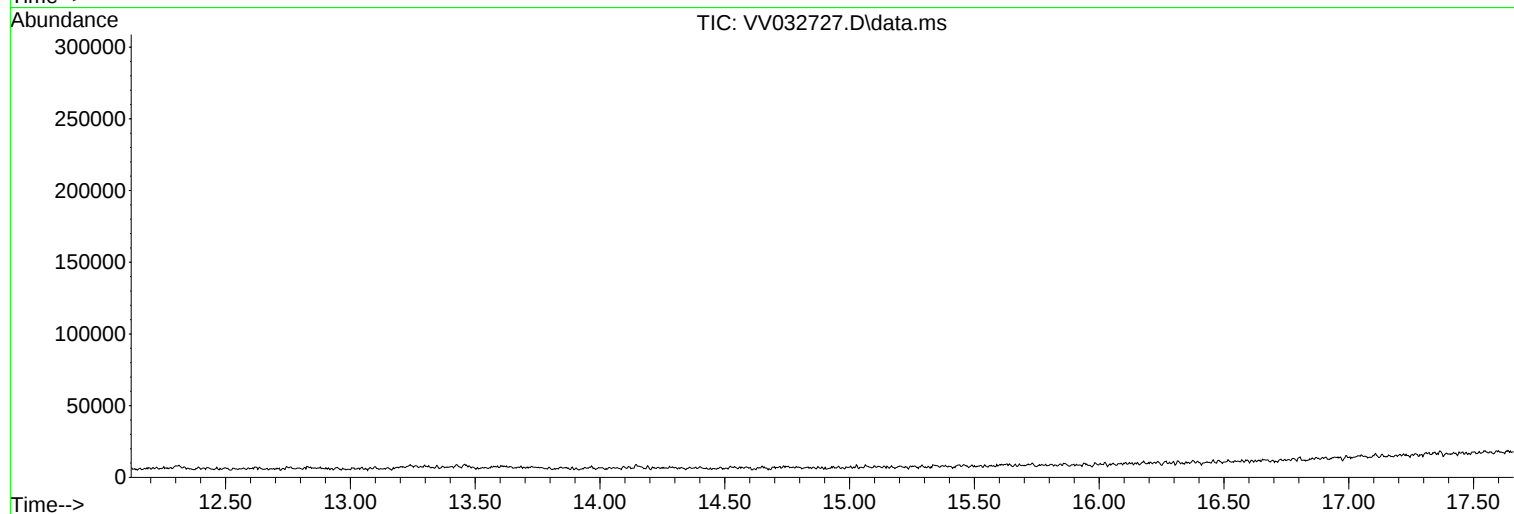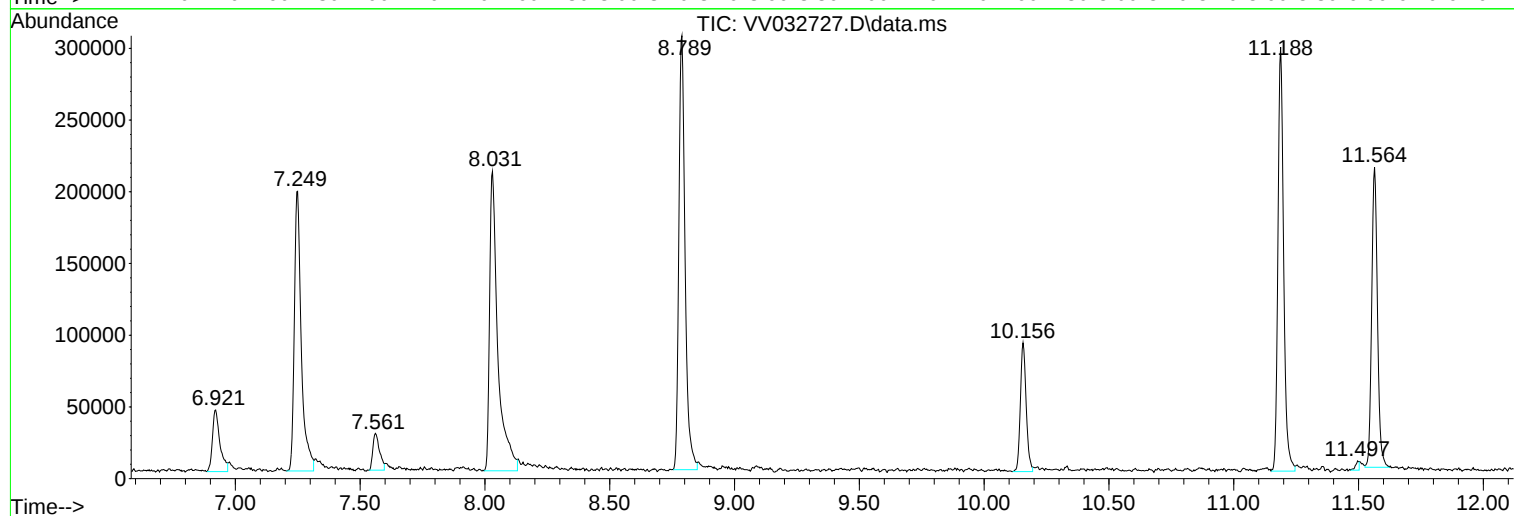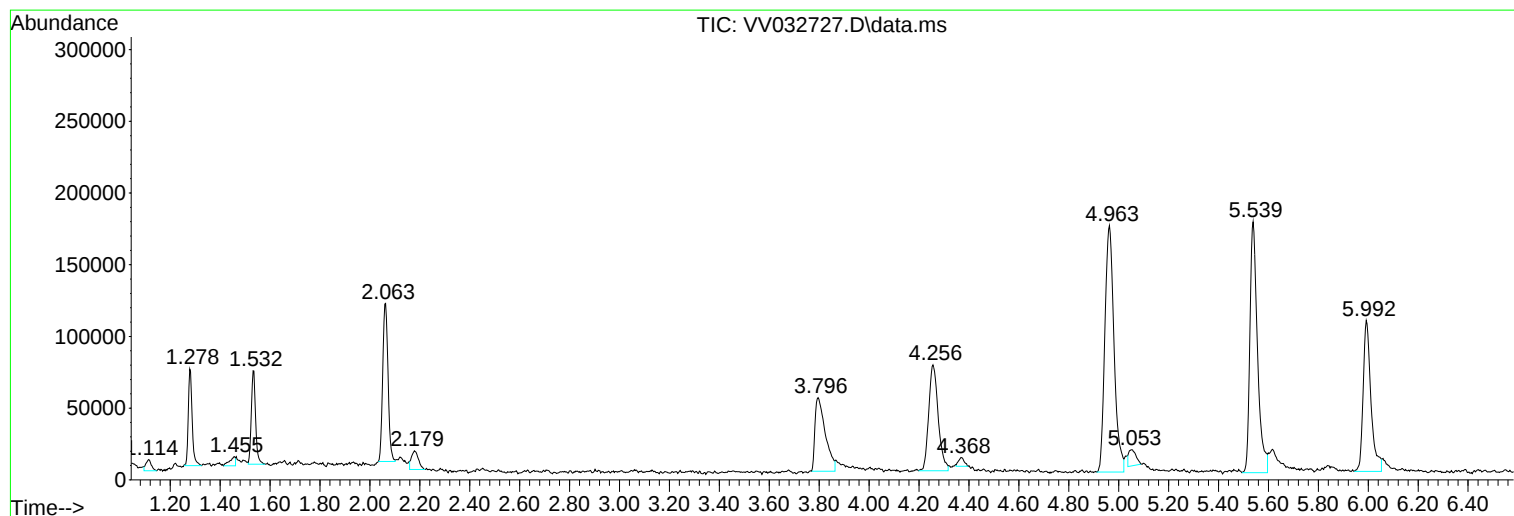

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032727.D
Acq On : 28 Oct 2023 09:05
Operator : SY/MD
Sample : 05019-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032727.D
Acq On : 28 Oct 2023 09:05
Operator : SY/MD
Sample : 05019-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc