

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032736.D
 Acq On : 28 Oct 2023 12:53
 Operator : SY/MD
 Sample : 04993-09DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	85	rBV	81436	93993	6.06%	1.554%
2	1.532	146	153	167	rVB	72340	84132	5.42%	1.391%
3	2.060	307	317	333	rVB	128520	184263	11.88%	3.046%
4	2.185	346	356	369	rVB3	18619	37247	2.40%	0.616%
5	3.818	853	864	889	rBV3	48904	189227	12.20%	3.128%
6	4.252	985	999	1020	rBV	84701	224566	14.48%	3.712%
7	4.960	1203	1219	1239	rBV2	199805	509390	32.84%	8.420%
8	5.538	1387	1399	1416	rBV	159616	337910	21.78%	5.586%
9	5.992	1526	1540	1555	rBV	119049	249136	16.06%	4.118%
10	6.918	1816	1828	1841	rBV	52481	102132	6.58%	1.688%
11	7.246	1919	1930	1952	rBV	225088	435973	28.10%	7.206%
12	7.561	2017	2028	2049	rBV4	29883	66074	4.26%	1.092%
13	7.905	2119	2135	2164	rBV	848316	1551287	100.00%	25.642%
14	8.030	2165	2174	2203	rBV	233889	511101	32.95%	8.448%
15	8.786	2399	2409	2430	rBV	276153	484099	31.21%	8.002%
16	10.156	2823	2835	2851	rBV	95835	160853	10.37%	2.659%
17	10.326	2880	2888	2897	rBV3	13604	21700	1.40%	0.359%
18	11.188	3143	3156	3177	rBV	266795	426675	27.50%	7.053%
19	11.564	3259	3273	3288	rBV	235450	379996	24.50%	6.281%




Sum of corrected areas: 6049754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032736.D
Acq On : 28 Oct 2023 12:53
Operator : SY/MD
Sample : 04993-09DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

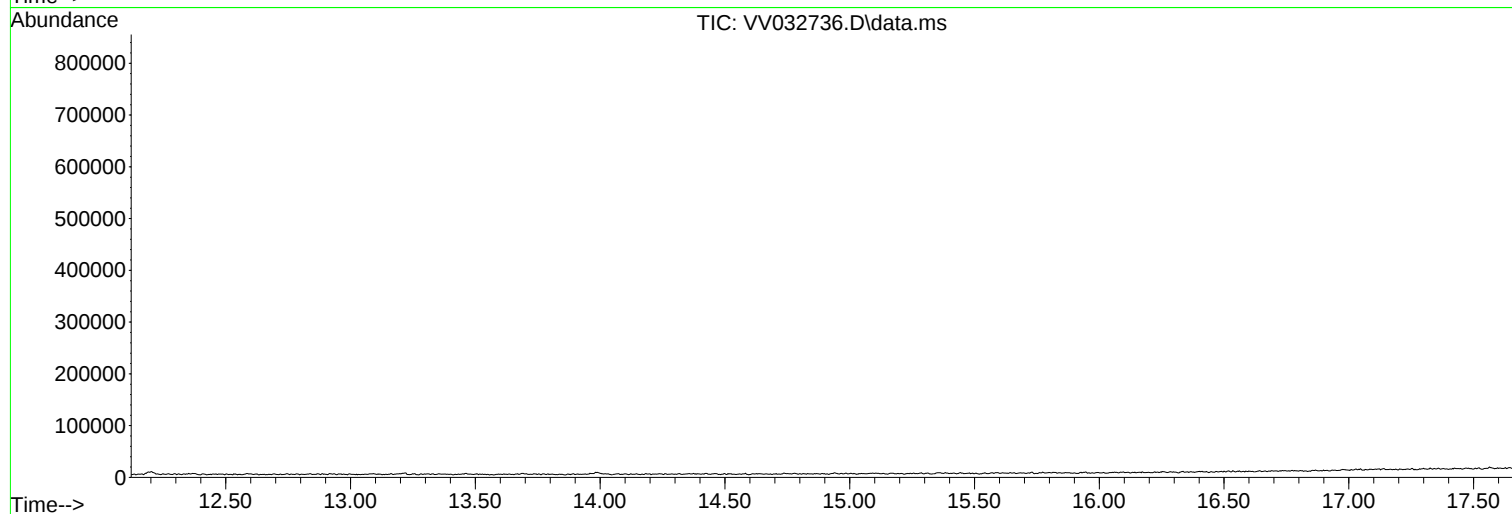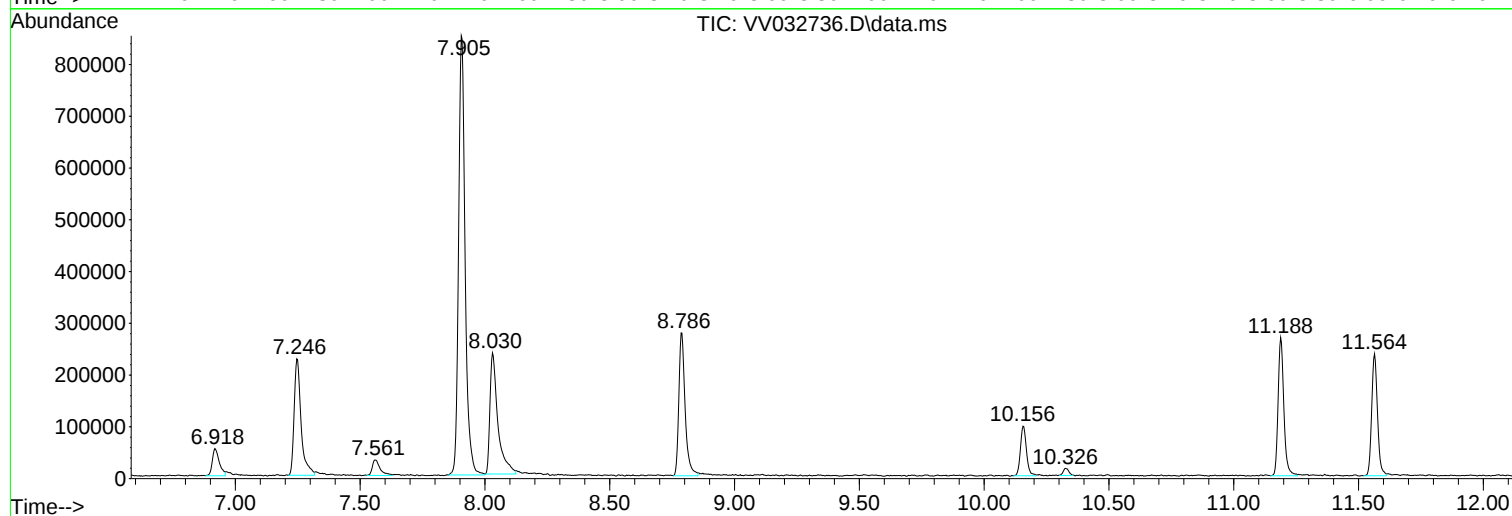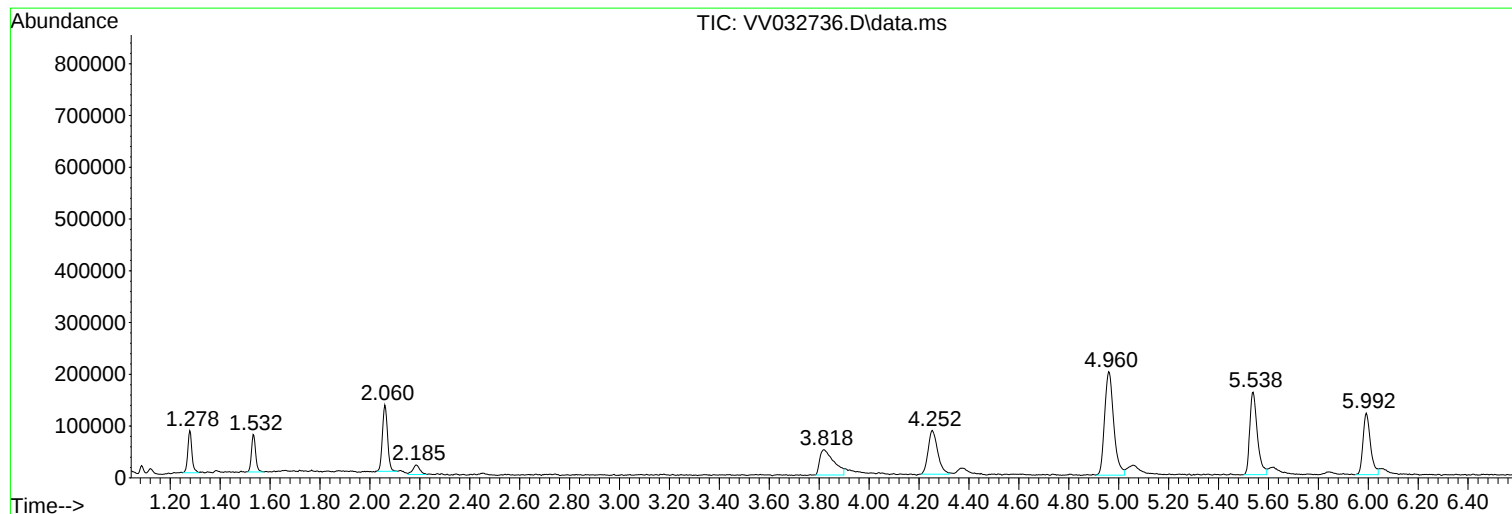

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032736.D
Acq On : 28 Oct 2023 12:53
Operator : SY/MD
Sample : 04993-09DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032736.D
Acq On : 28 Oct 2023 12:53
Operator : SY/MD
Sample : 04993-09DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------