

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032737.D
 Acq On : 28 Oct 2023 13:17
 Operator : SY/MD
 Sample : 04993-19 25X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	86	rBV	75006	85325	7.60%	1.527%
2	1.532	146	153	162	rBV	69167	80903	7.20%	1.448%
3	2.060	304	317	329	rBV	128567	188392	16.77%	3.371%
4	2.188	349	357	366	rVB2	17996	29855	2.66%	0.534%
5	3.819	849	864	903	rBV2	52822	242276	21.57%	4.335%
6	4.253	983	999	1020	rBV	85365	222743	19.83%	3.986%
7	4.378	1028	1038	1055	rVB4	12411	32010	2.85%	0.573%
8	4.960	1204	1219	1239	rBV4	194992	494225	44.00%	8.843%
9	5.539	1384	1399	1416	rBV	151437	324675	28.90%	5.810%
10	5.992	1526	1540	1555	rBV2	115273	247152	22.00%	4.422%
11	6.918	1818	1828	1850	rBV3	47643	104004	9.26%	1.861%
12	7.246	1920	1930	1957	rBV	217607	433376	38.58%	7.755%
13	7.561	2018	2028	2040	rBV2	29513	60284	5.37%	1.079%
14	7.905	2121	2135	2158	rBV	619999	1123321	100.00%	20.100%
15	8.031	2164	2174	2206	rBV	228689	508784	45.29%	9.104%
16	8.789	2399	2410	2430	rBV	260032	458881	40.85%	8.211%
17	10.156	2825	2835	2850	rBV2	94007	151837	13.52%	2.717%
18	10.326	2879	2888	2898	rBV7	6553	13521	1.20%	0.242%
19	11.188	3144	3156	3175	rBV	255509	412029	36.68%	7.373%
20	11.564	3261	3273	3287	rBV	229633	375034	33.39%	6.711%




Sum of corrected areas: 5588627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032737.D
Acq On : 28 Oct 2023 13:17
Operator : SY/MD
Sample : 04993-19 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

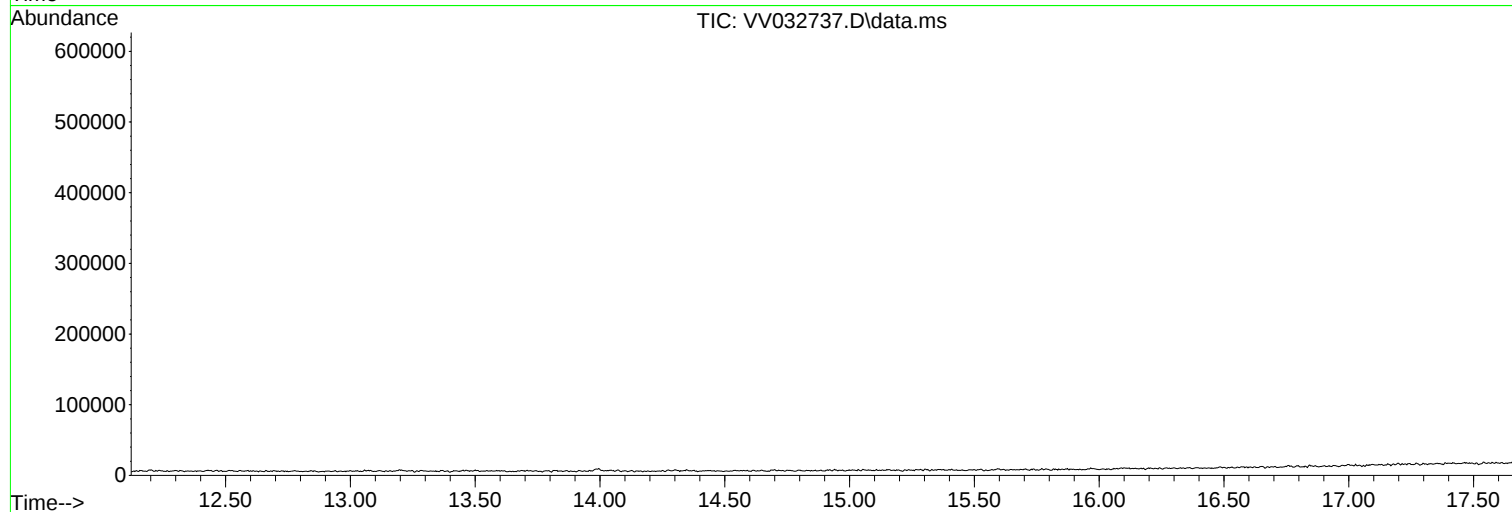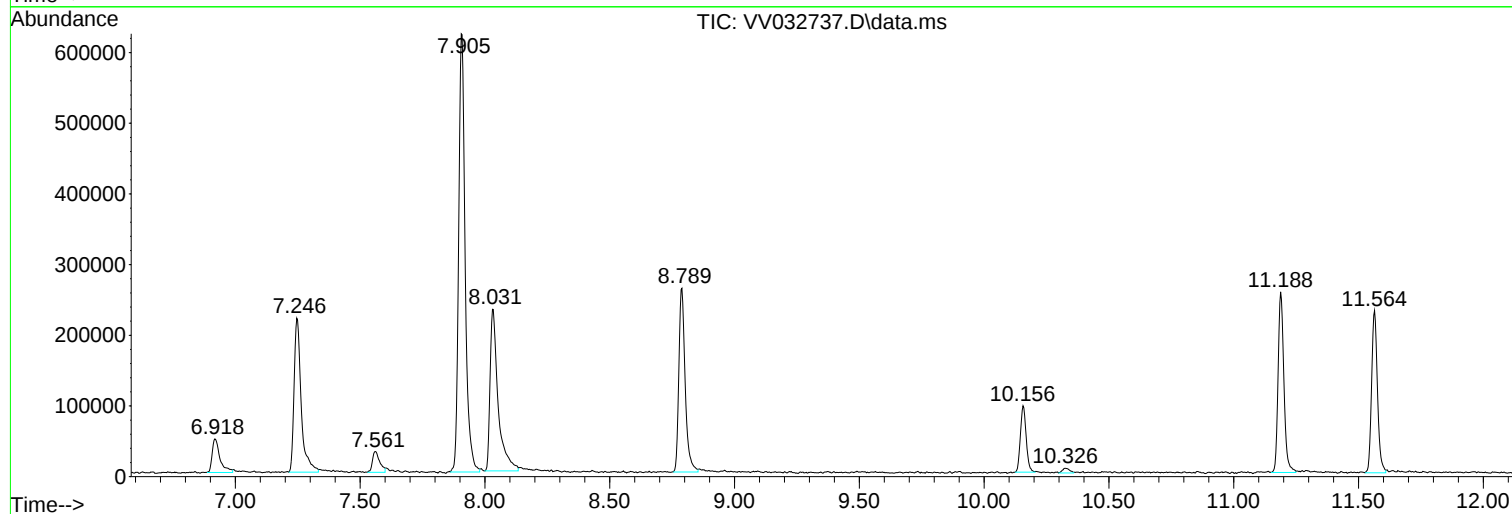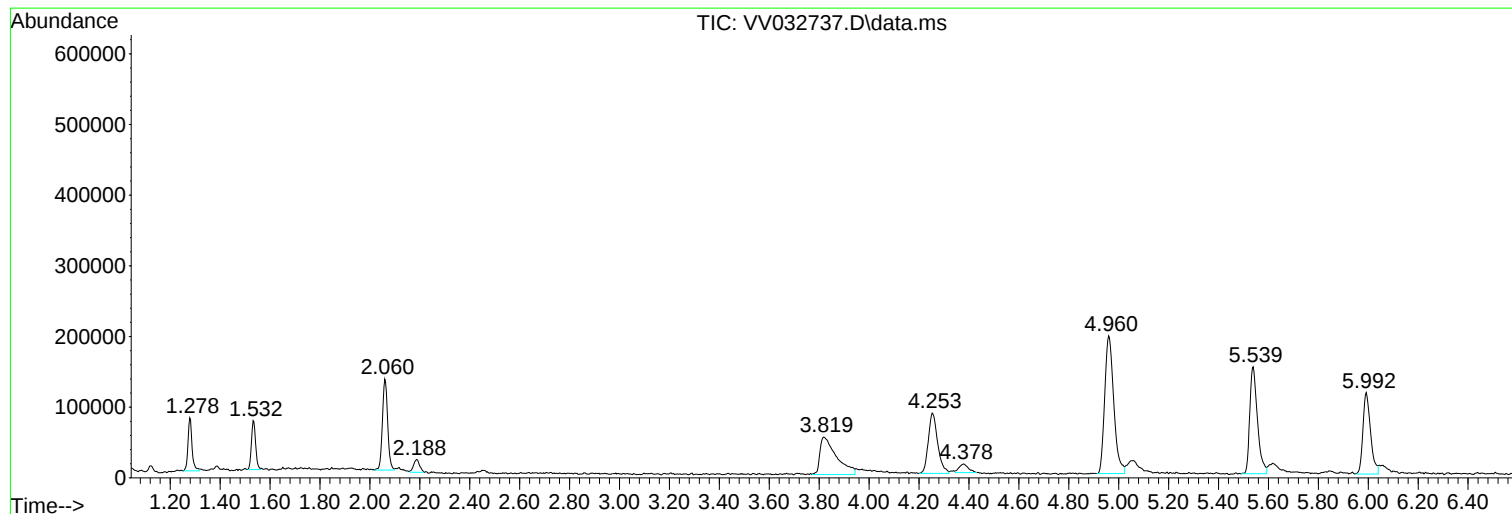

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032737.D
Acq On : 28 Oct 2023 13:17
Operator : SY/MD
Sample : 04993-19 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032737.D
Acq On : 28 Oct 2023 13:17
Operator : SY/MD
Sample : 04993-19 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 69 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc