

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032738.D
 Acq On : 28 Oct 2023 13:39
 Operator : SY/MD
 Sample : 04993-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	86	rBV	78067	83016	1.37%	0.810%
2	1.532	145	153	163	rBV	65702	79900	1.32%	0.779%
3	2.060	307	317	332	rBV	121749	179524	2.96%	1.751%
4	3.819	854	864	895	rBV2	47067	181252	2.98%	1.768%
5	4.256	986	1000	1021	rBV3	81983	213339	3.51%	2.081%
6	4.960	1205	1219	1238	rBV3	184281	466576	7.68%	4.551%
7	5.539	1388	1399	1416	rBV	150207	313248	5.16%	3.056%
8	5.992	1528	1540	1554	rBV	109630	227347	3.74%	2.218%
9	6.918	1819	1828	1841	rBV2	46753	96942	1.60%	0.946%
10	7.249	1918	1931	1957	rBV	211781	422744	6.96%	4.124%
11	7.905	2116	2135	2162	rBV	3420229	6074445	100.00%	59.255%
12	8.031	2165	2174	2209	rVB	240183	517529	8.52%	5.048%
13	8.789	2395	2410	2431	rBV	262730	469689	7.73%	4.582%
14	10.156	2824	2835	2852	rBV	88562	151085	2.49%	1.474%
15	11.188	3144	3156	3171	rBV	251685	407192	6.70%	3.972%
16	11.564	3261	3273	3294	rBV	219276	367554	6.05%	3.585%




Sum of corrected areas: 10251382

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032738.D
Acq On : 28 Oct 2023 13:39
Operator : SY/MD
Sample : 04993-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

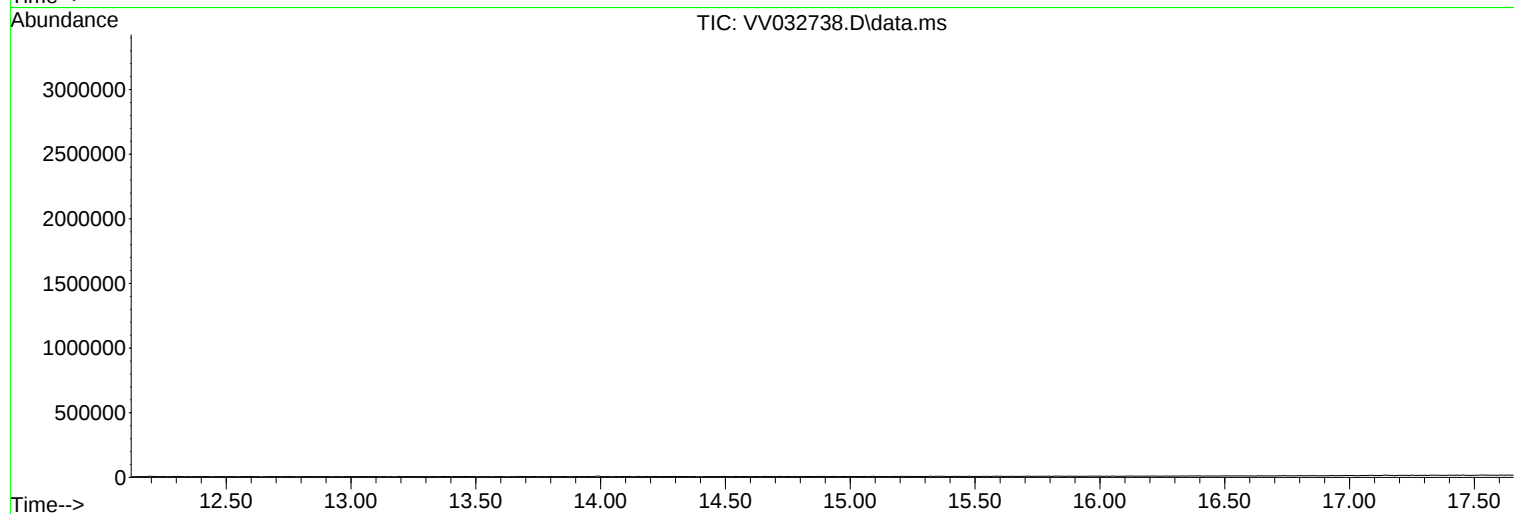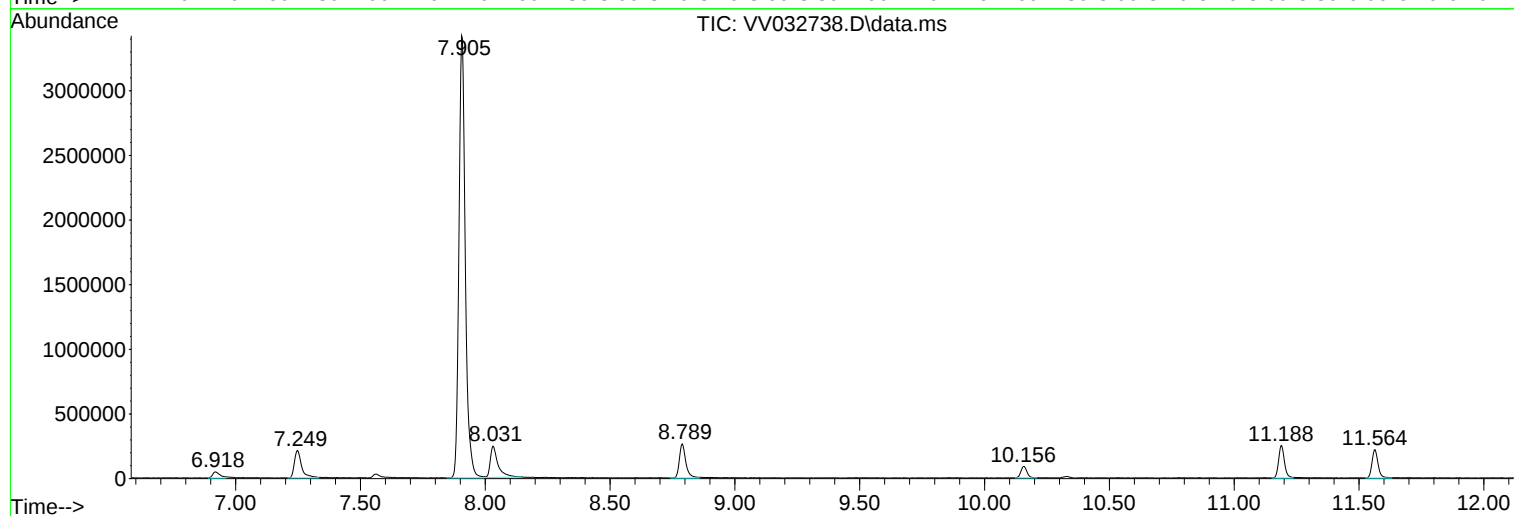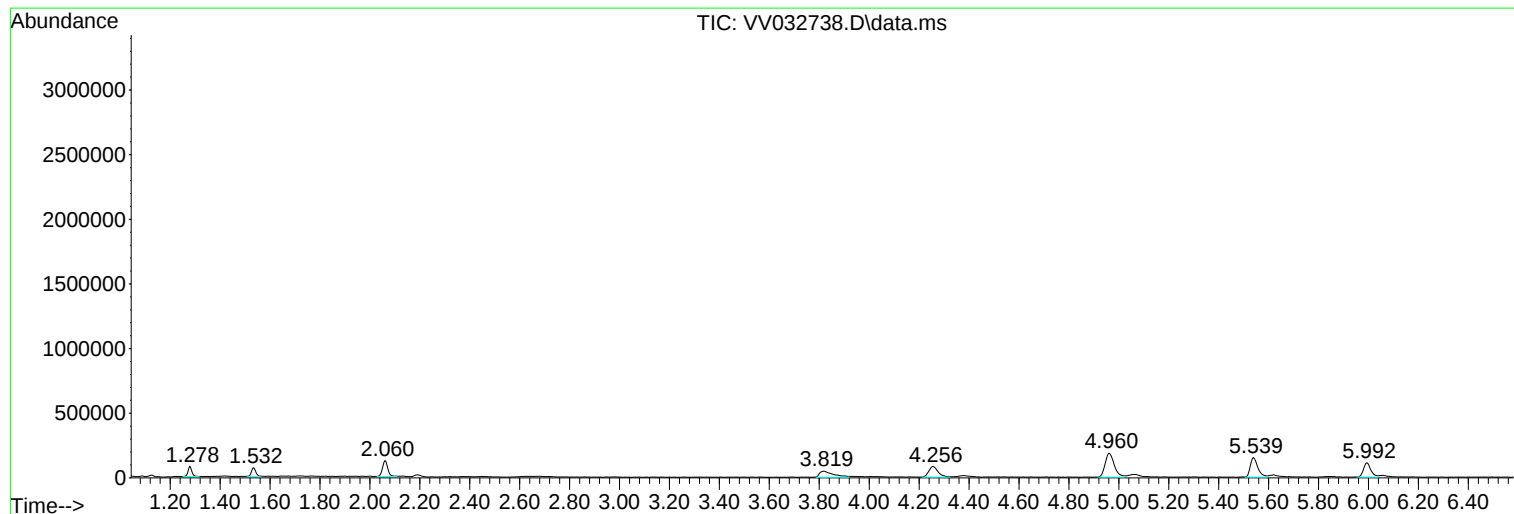

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032738.D
Acq On : 28 Oct 2023 13:39
Operator : SY/MD
Sample : 04993-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032738.D
Acq On : 28 Oct 2023 13:39
Operator : SY/MD
Sample : 04993-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc