

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032740.D
 Acq On : 28 Oct 2023 14:28
 Operator : SY/MD
 Sample : 05019-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4919

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032740.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	20	27	34	rVB	7252	11461	2.24%	0.252%
2	1.217	44	55	63	rBV	10048	16207	3.16%	0.357%
3	1.278	65	74	87	rBV	81713	88908	17.36%	1.956%
4	1.532	143	153	165	rBV	76044	92819	18.12%	2.042%
5	2.059	308	317	331	rBV	127994	185841	36.28%	4.089%
6	2.191	348	358	369	rVB	17750	31679	6.18%	0.697%
7	3.805	850	860	889	rBV2	56627	189655	37.02%	4.173%
8	4.252	985	999	1026	rBV	84148	224510	43.83%	4.940%
9	4.378	1026	1038	1052	rVB5	11873	31379	6.13%	0.690%
10	4.960	1204	1219	1238	rBV2	201435	512263	100.00%	11.271%
11	5.538	1386	1399	1417	rBV2	151545	323310	63.11%	7.113%
12	5.619	1417	1424	1437	rVB3	10838	24573	4.80%	0.541%
13	5.992	1526	1540	1554	rBV	121299	257903	50.35%	5.674%
14	6.918	1818	1828	1843	rBV2	52917	104928	20.48%	2.309%
15	7.246	1918	1930	1950	rBV	233300	443758	86.63%	9.764%
16	7.561	2015	2028	2047	rBV2	32803	71197	13.90%	1.566%
17	8.030	2164	2174	2203	rBV	234424	505741	98.73%	11.127%
18	8.789	2395	2410	2434	rBV	261359	462074	90.20%	10.167%
19	9.078	2490	2500	2501	rBV9	8105	7639	1.49%	0.168%
20	10.156	2825	2835	2848	rBV	93641	156783	30.61%	3.450%
21	10.329	2881	2889	2898	rBV	6585	12731	2.49%	0.280%
22	11.188	3146	3156	3173	rBV	253837	411574	80.34%	9.055%
23	11.564	3261	3273	3290	rBV	236788	378109	73.81%	8.319%




Sum of corrected areas: 4545042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032740.D
Acq On : 28 Oct 2023 14:28
Operator : SY/MD
Sample : 05019-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

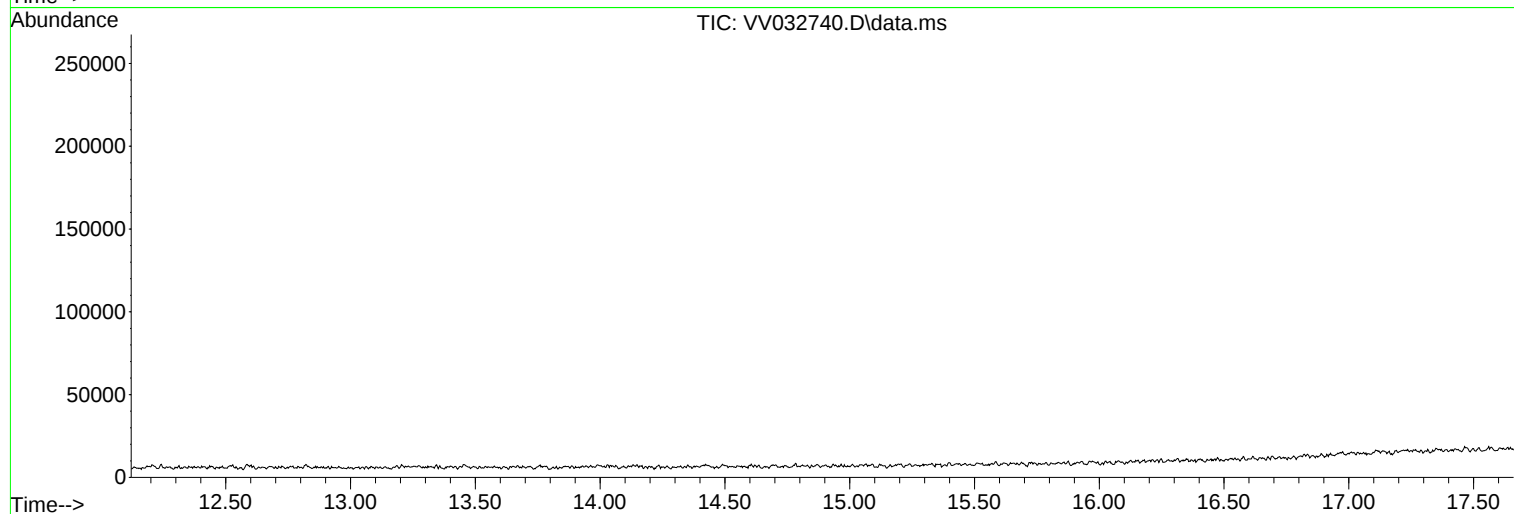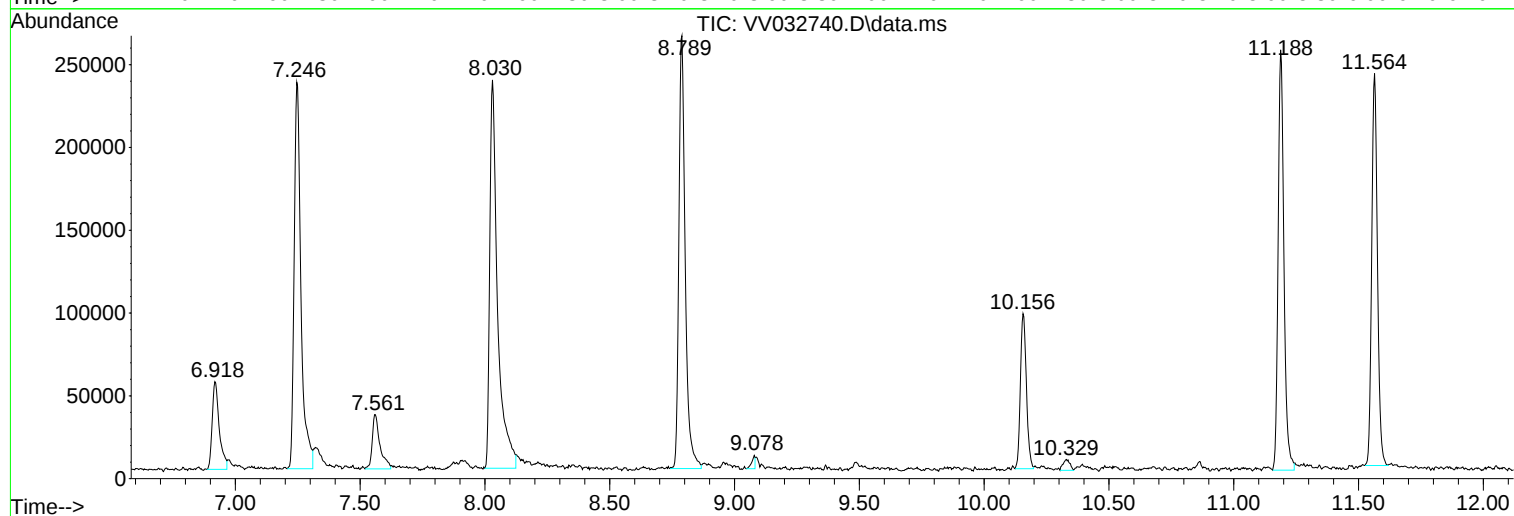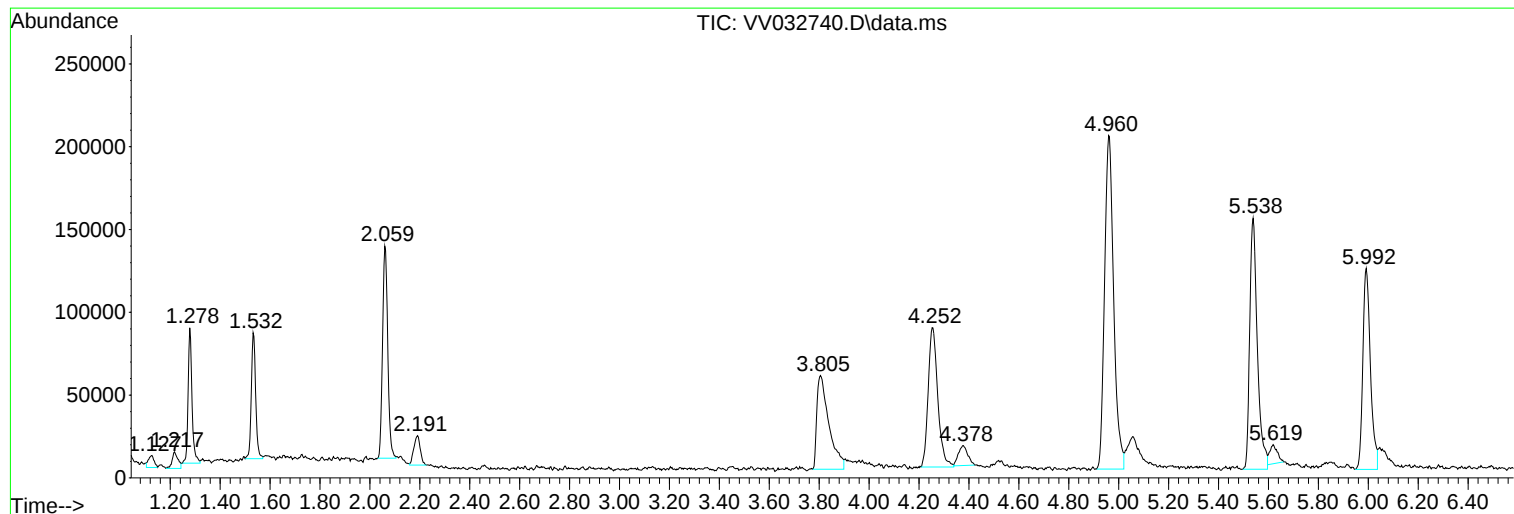

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032740.D
Acq On : 28 Oct 2023 14:28
Operator : SY/MD
Sample : 05019-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032740.D
Acq On : 28 Oct 2023 14:28
Operator : SY/MD
Sample : 05019-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc