

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032743.D
 Acq On : 28 Oct 2023 15:41
 Operator : SY/MD
 Sample : 05019-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49H7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	33	rVB	6849	8157	1.66%	0.189%
2	1.220	49	56	60	rBV8	5392	7371	1.50%	0.171%
3	1.278	68	74	84	rBV	72943	75877	15.47%	1.755%
4	1.532	145	153	162	rBV	75122	89820	18.31%	2.078%
5	2.060	307	317	331	rVB	120987	176791	36.05%	4.090%
6	2.188	350	357	368	rVB3	17850	29902	6.10%	0.692%
7	3.802	851	859	886	rBV	52696	164955	33.63%	3.816%
8	4.256	985	1000	1019	rBV	78928	206129	42.03%	4.769%
9	4.381	1023	1039	1052	rVV2	12523	31880	6.50%	0.738%
10	4.960	1200	1219	1239	rBV2	188307	490454	100.00%	11.346%
11	5.056	1243	1249	1251	rBV6	6887	7966	1.62%	0.184%
12	5.539	1385	1399	1415	rBV	146550	313415	63.90%	7.250%
13	5.619	1420	1424	1436	rVB2	9660	18047	3.68%	0.417%
14	5.992	1528	1540	1554	rBV2	111799	233284	47.56%	5.397%
15	6.918	1816	1828	1841	rBV	50477	98218	20.03%	2.272%
16	7.246	1919	1930	1953	rBV	214871	417511	85.13%	9.659%
17	7.561	2019	2028	2046	rBV3	29502	62013	12.64%	1.435%
18	8.030	2163	2174	2213	rBV	213912	489499	99.81%	11.324%
19	8.789	2397	2410	2431	rBV	259735	453394	92.44%	10.489%
20	9.085	2495	2502	2511	rBV9	5979	9809	2.00%	0.227%
21	10.156	2824	2835	2854	rBV2	92613	155176	31.64%	3.590%
22	10.326	2881	2888	2896	rVB2	5477	9408	1.92%	0.218%
23	10.860	3046	3054	3061	rBV10	4921	7621	1.55%	0.176%
24	11.188	3146	3156	3176	rBV	247094	394171	80.37%	9.119%
25	11.493	3243	3251	3252	rBV6	6879	7097	1.45%	0.164%
26	11.564	3262	3273	3294	rVB	225133	364714	74.36%	8.437%




Sum of corrected areas: 4322679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032743.D
Acq On : 28 Oct 2023 15:41
Operator : SY/MD
Sample : 05019-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

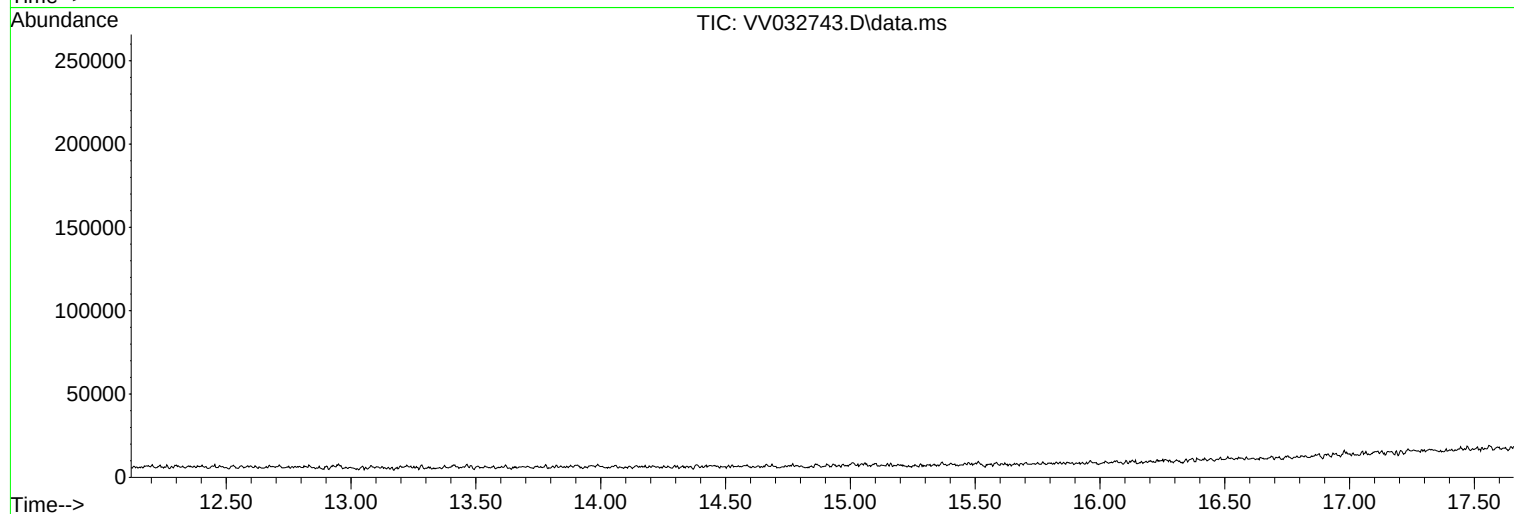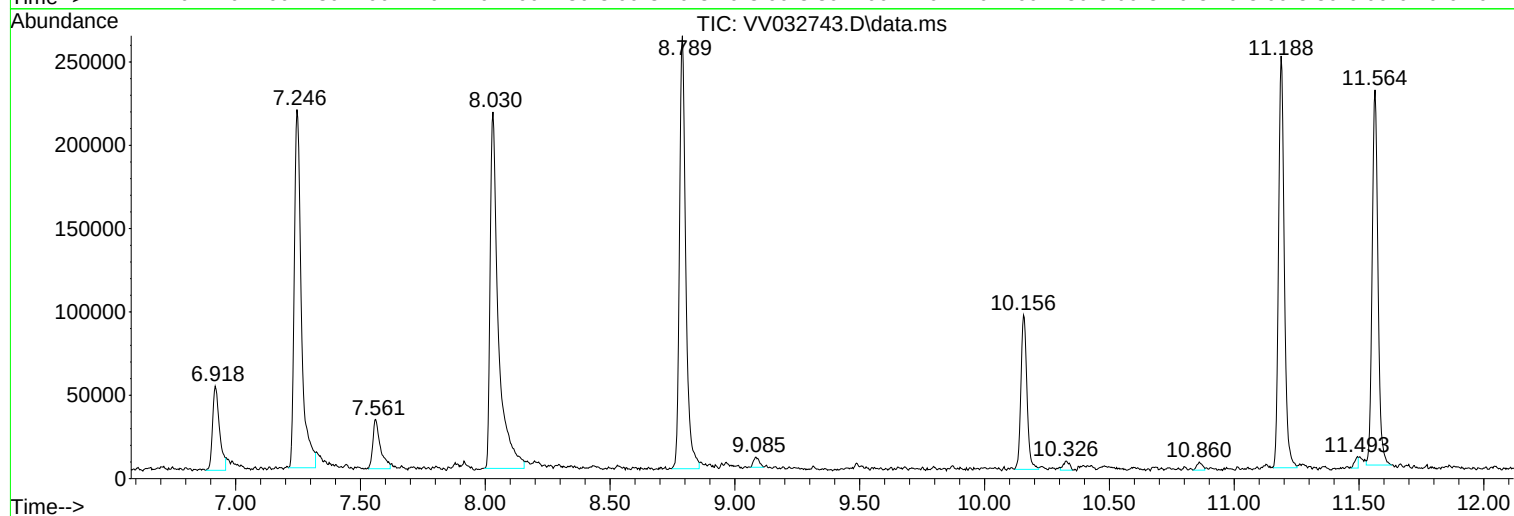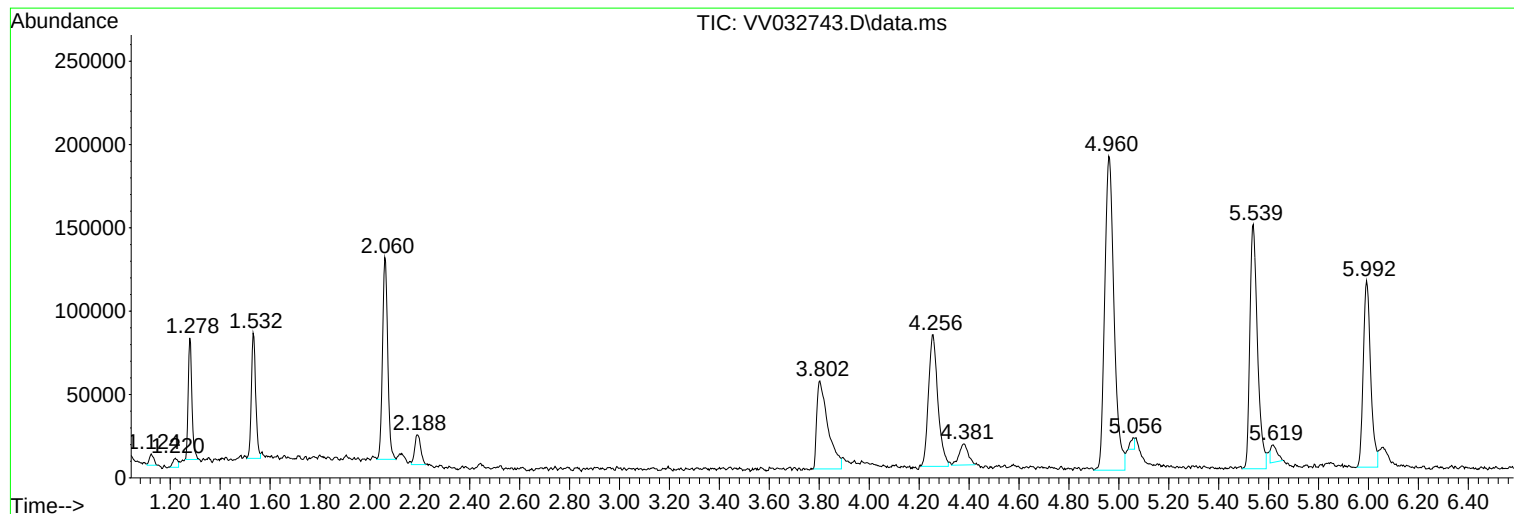

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032743.D
Acq On : 28 Oct 2023 15:41
Operator : SY/MD
Sample : 05019-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032743.D
Acq On : 28 Oct 2023 15:41
Operator : SY/MD
Sample : 05019-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49H7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------