

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032748.D
 Acq On : 28 Oct 2023 17:43
 Operator : SY/MD
 Sample : 05103-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49W9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	23	27	34	rVB	7092	8409	1.76%	0.194%
2	1.278	68	74	88	rVB	74550	79699	16.63%	1.841%
3	1.532	146	153	166	rVB	73218	84419	17.62%	1.950%
4	2.059	308	317	328	rBV	121391	179302	37.42%	4.142%
5	2.191	346	358	369	rVB2	17765	35562	7.42%	0.821%
6	3.805	850	860	892	rBV2	50610	166862	34.83%	3.855%
7	4.252	983	999	1018	rBV	78739	211684	44.18%	4.890%
8	4.371	1028	1036	1051	rVB3	11728	29542	6.17%	0.682%
9	4.960	1205	1219	1237	rBV4	186317	475751	99.30%	10.990%
10	5.050	1242	1247	1249	rBV6	6733	6839	1.43%	0.158%
11	5.538	1386	1399	1417	rBV	151027	323914	67.61%	7.483%
12	5.841	1483	1493	1503	rBV	4429	9311	1.94%	0.215%
13	5.992	1527	1540	1554	rBV	110762	235557	49.17%	5.441%
14	6.918	1819	1828	1840	rBV2	46158	89471	18.67%	2.067%
15	7.246	1919	1930	1949	rBV	214098	408436	85.25%	9.435%
16	7.561	2017	2028	2038	rBV2	29975	56920	11.88%	1.315%
17	8.030	2164	2174	2205	rBV	216347	479107	100.00%	11.068%
18	8.789	2397	2410	2436	rBV	261701	468951	97.88%	10.833%
19	9.085	2494	2502	2512	rBV2	9462	15019	3.13%	0.347%
20	9.490	2620	2628	2636	rBV10	6025	9983	2.08%	0.231%
21	10.156	2825	2835	2849	rBV	92729	152149	31.76%	3.515%
22	10.329	2883	2889	2898	rVB	5509	8639	1.80%	0.200%
23	10.863	3046	3055	3066	rBV	6489	10777	2.25%	0.249%
24	11.188	3144	3156	3172	rBV	254359	408328	85.23%	9.433%
25	11.503	3243	3254	3260	rBV	5386	11988	2.50%	0.277%
26	11.564	3262	3273	3288	rVV	223417	362306	75.62%	8.369%




Sum of corrected areas: 4328925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032748.D
Acq On : 28 Oct 2023 17:43
Operator : SY/MD
Sample : 05103-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49W9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

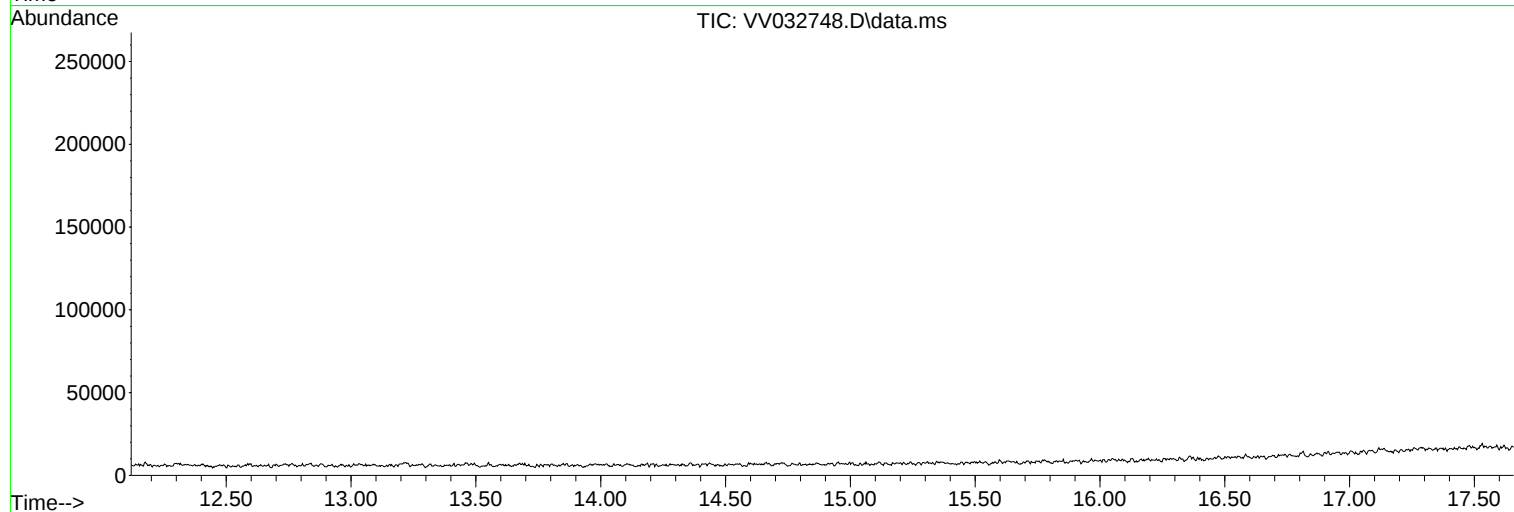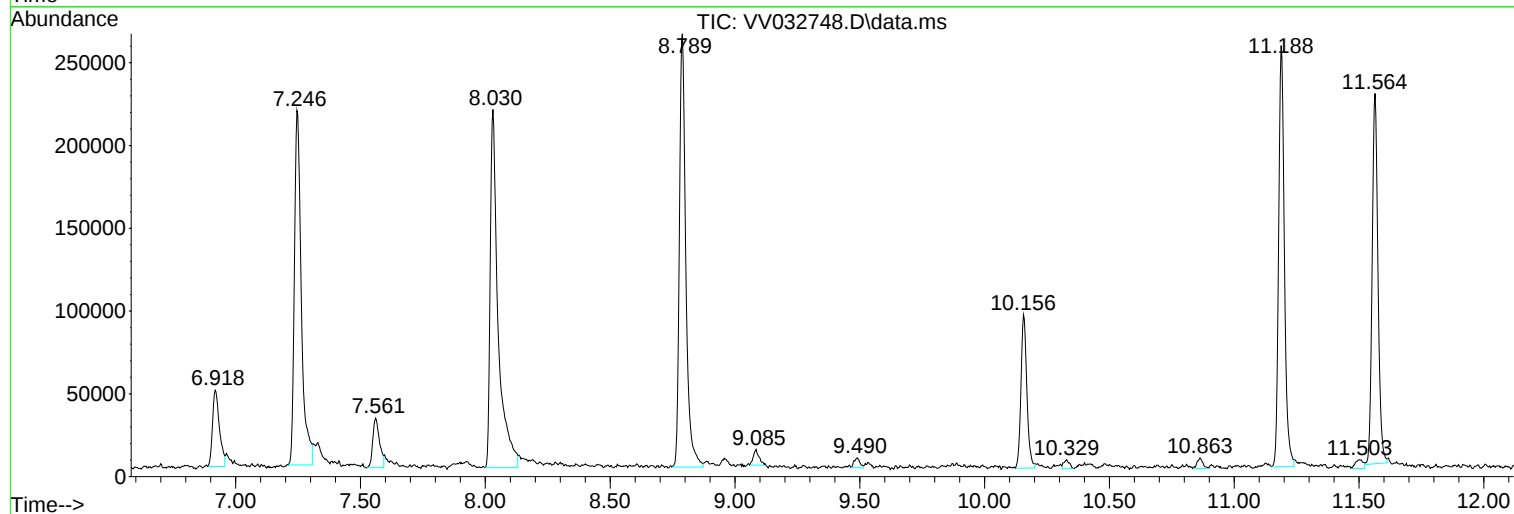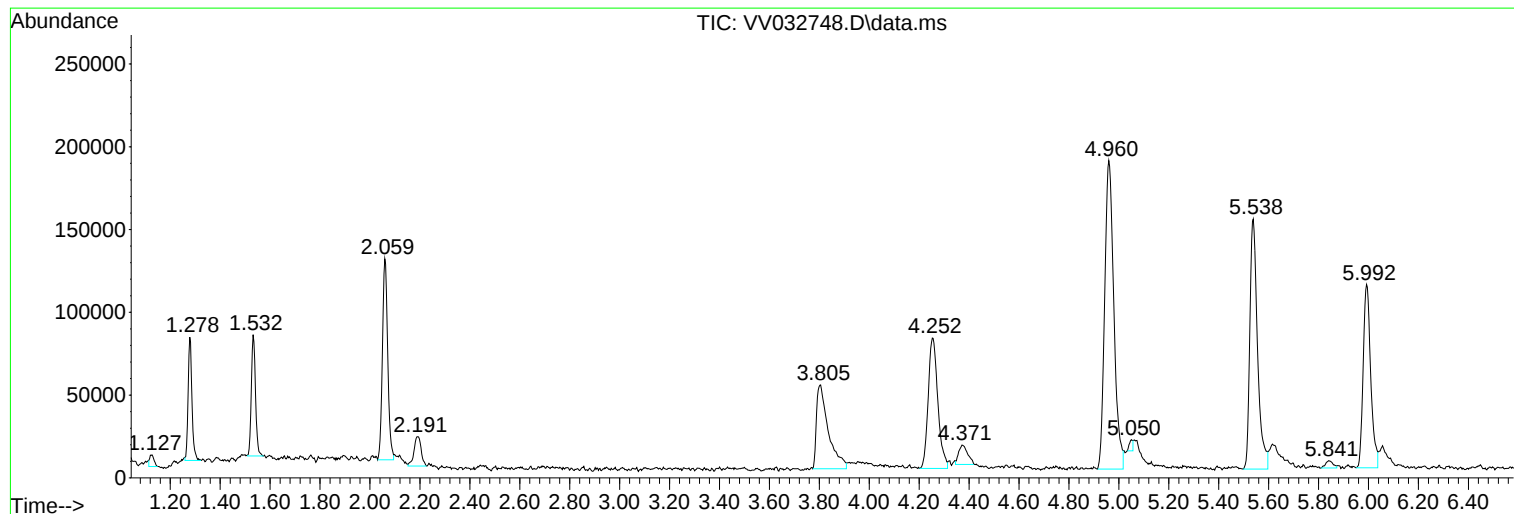

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032748.D
Acq On : 28 Oct 2023 17:43
Operator : SY/MD
Sample : 05103-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49W9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032748.D
Acq On : 28 Oct 2023 17:43
Operator : SY/MD
Sample : 05103-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 80 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49W9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc