

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032750.D
 Acq On : 28 Oct 2023 18:32
 Operator : SY/MD
 Sample : 05103-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49X5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	16	26	36	rVB2	7367	12902	2.61%	0.295%
2	1.214	50	54	65	rBV	7714	11175	2.26%	0.256%
3	1.278	65	74	86	rBV	76239	84848	17.16%	1.943%
4	1.532	147	153	164	rVB	71220	82817	16.75%	1.897%
5	2.059	307	317	332	rBV	120868	179395	36.29%	4.108%
6	2.191	349	358	371	rVB2	19208	36081	7.30%	0.826%
7	3.802	849	859	885	rBV	54788	172997	35.00%	3.962%
8	4.256	984	1000	1021	rBV2	77910	206697	41.81%	4.734%
9	4.378	1024	1038	1047	rBV3	12663	31003	6.27%	0.710%
10	4.960	1203	1219	1239	rBV4	186854	488120	98.75%	11.179%
11	5.053	1242	1248	1268	rVB7	17570	49833	10.08%	1.141%
12	5.538	1386	1399	1415	rBV	148749	315627	63.85%	7.228%
13	5.992	1527	1540	1554	rBV	111471	235345	47.61%	5.390%
14	6.918	1817	1828	1845	rBV2	48026	98351	19.90%	2.252%
15	7.246	1920	1930	1961	rBV	211857	416623	84.28%	9.541%
16	7.561	2018	2028	2043	rBV2	29279	56300	11.39%	1.289%
17	8.030	2161	2174	2212	rBV2	213340	494315	100.00%	11.321%
18	8.789	2397	2410	2439	rBV	263743	478919	96.89%	10.968%
19	10.156	2825	2835	2850	rBV2	91057	149232	30.19%	3.418%
20	11.188	3145	3156	3173	rBV	254756	401740	81.27%	9.200%
21	11.564	3262	3273	3292	rVB	222133	364217	73.68%	8.341%




Sum of corrected areas: 4366537

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032750.D
Acq On : 28 Oct 2023 18:32
Operator : SY/MD
Sample : 05103-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

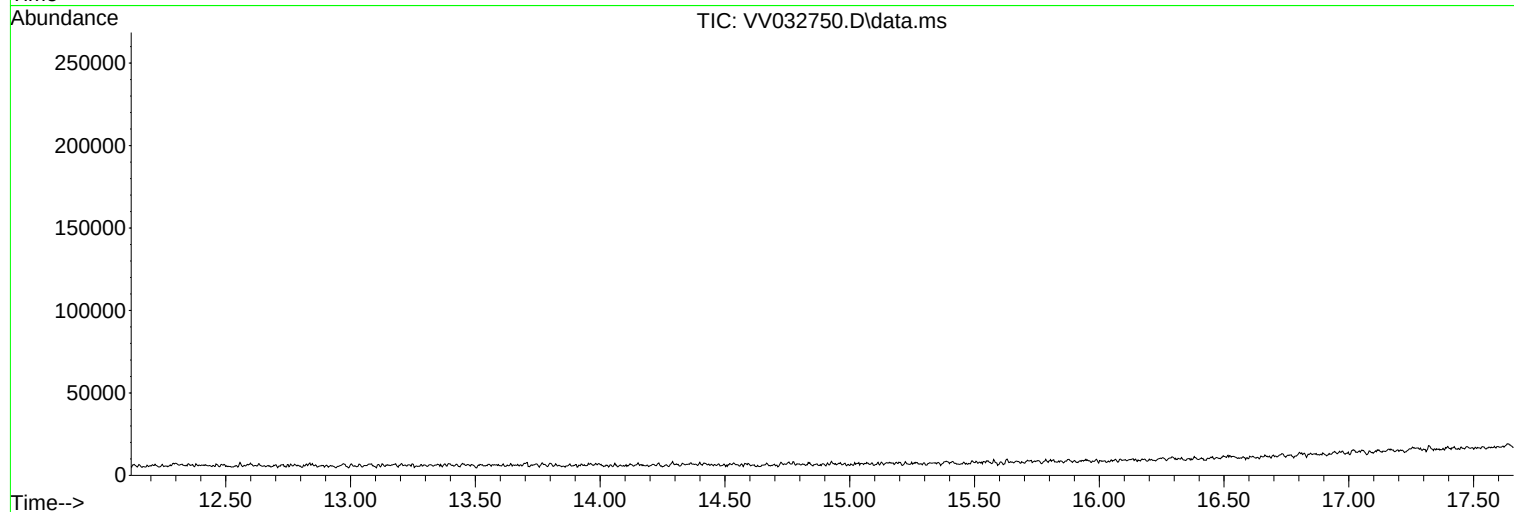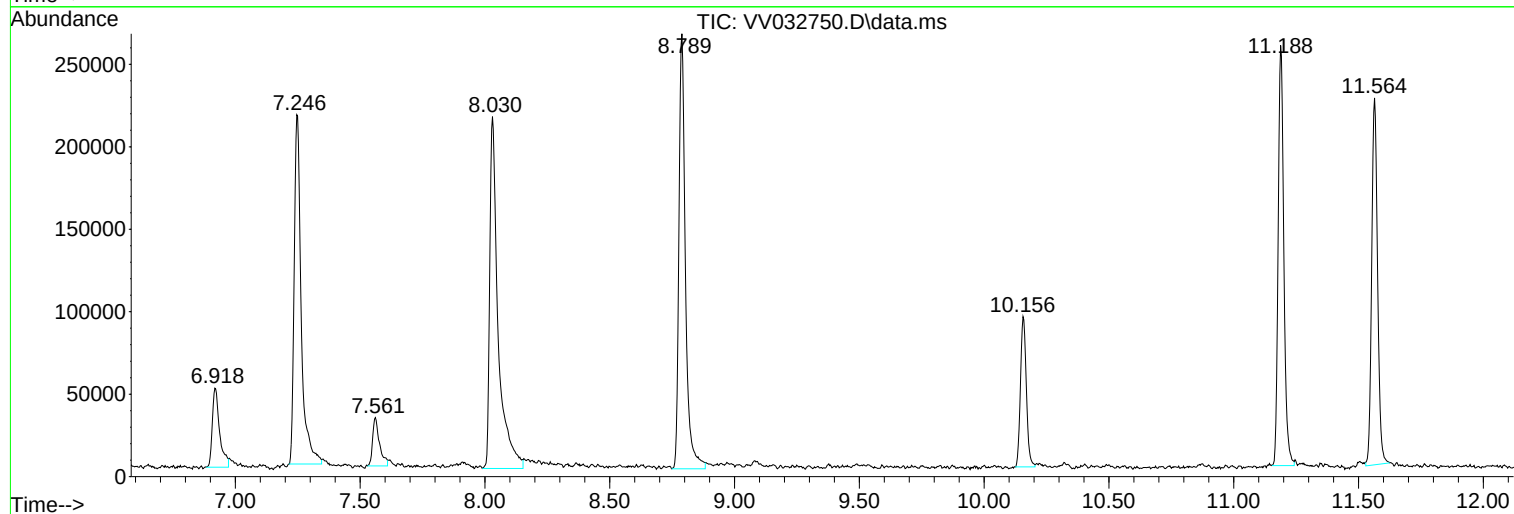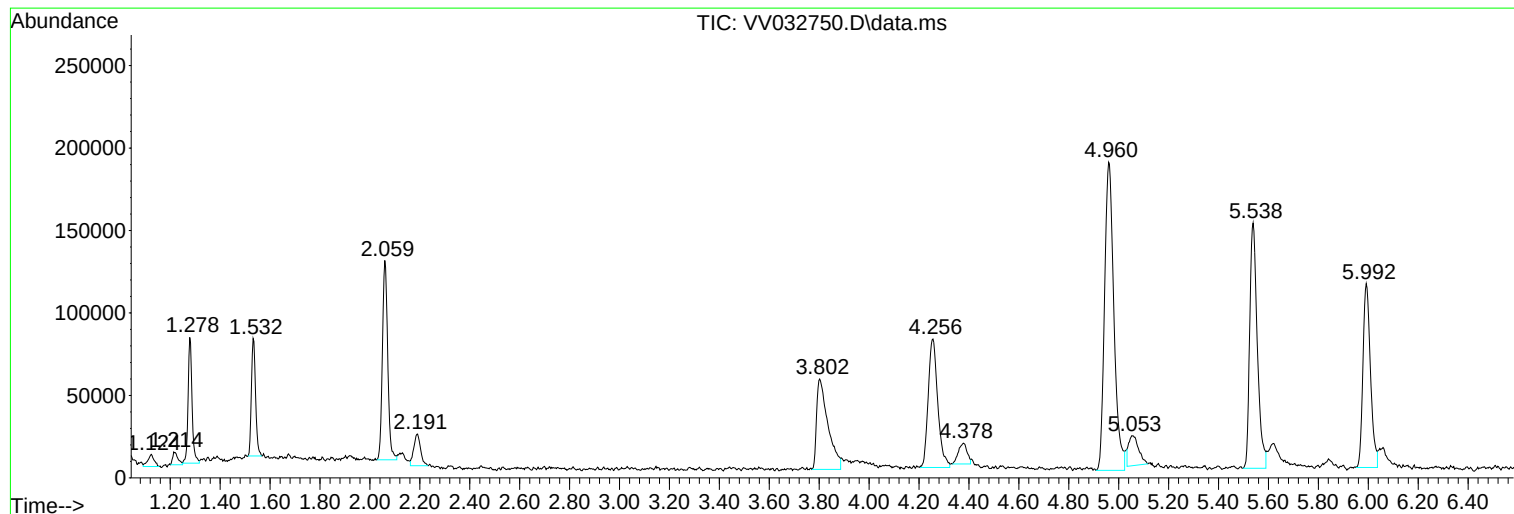

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032750.D
Acq On : 28 Oct 2023 18:32
Operator : SY/MD
Sample : 05103-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032750.D
Acq On : 28 Oct 2023 18:32
Operator : SY/MD
Sample : 05103-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------