

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032751.D
 Acq On : 28 Oct 2023 18:56
 Operator : SY/MD
 Sample : 05103-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49X6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032751.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	22	27	36	rVB	7256	8973	1.81%	0.206%
2	1.278	67	74	85	rBV	74410	81149	16.39%	1.859%
3	1.532	141	153	164	rBV	75799	94345	19.05%	2.161%
4	2.060	309	317	332	rVB	122207	175852	35.51%	4.028%
5	2.191	349	358	370	rVB2	16707	28668	5.79%	0.657%
6	3.802	851	859	886	rBV2	52958	174198	35.18%	3.990%
7	4.256	984	1000	1022	rBV3	79851	218115	44.05%	4.996%
8	4.378	1027	1038	1049	rVV3	10770	27432	5.54%	0.628%
9	4.960	1202	1219	1239	rBV3	191808	495197	100.00%	11.342%
10	5.059	1242	1250	1267	rVB6	16690	45970	9.28%	1.053%
11	5.539	1387	1399	1417	rBV2	147530	316734	63.96%	7.254%
12	5.992	1526	1540	1555	rBV	115074	245852	49.65%	5.631%
13	6.918	1818	1828	1842	rBV	47048	92076	18.59%	2.109%
14	7.246	1919	1930	1948	rBV	219285	421965	85.21%	9.665%
15	7.561	2020	2028	2046	rBV2	29435	61963	12.51%	1.419%
16	8.030	2164	2174	2207	rBV	217038	487619	98.47%	11.168%
17	8.789	2400	2410	2431	rBV	259445	453926	91.67%	10.397%
18	9.091	2494	2504	2509	rBV6	6505	11194	2.26%	0.256%
19	9.484	2620	2626	2631	rBV10	4862	5800	1.17%	0.133%
20	10.156	2822	2835	2855	rBV	95364	158208	31.95%	3.624%
21	11.188	3144	3156	3171	rBV	248317	396692	80.11%	9.086%
22	11.564	3262	3273	3290	rBV	229573	364177	73.54%	8.341%




Sum of corrected areas: 4366105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032751.D
Acq On : 28 Oct 2023 18:56
Operator : SY/MD
Sample : 05103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

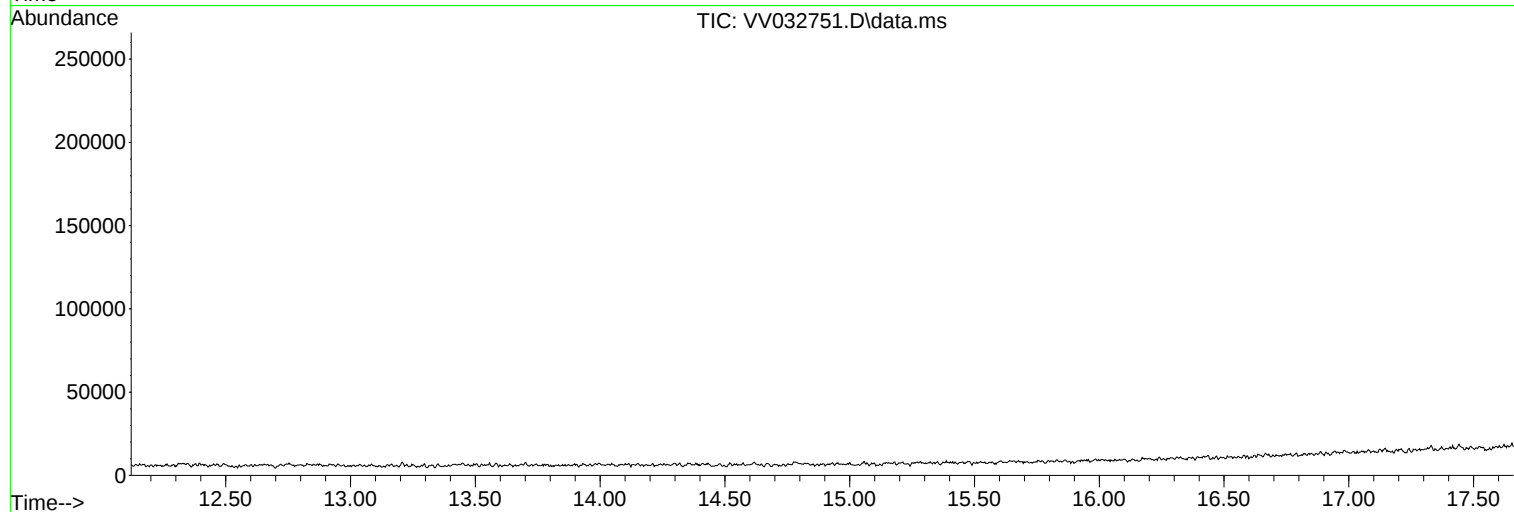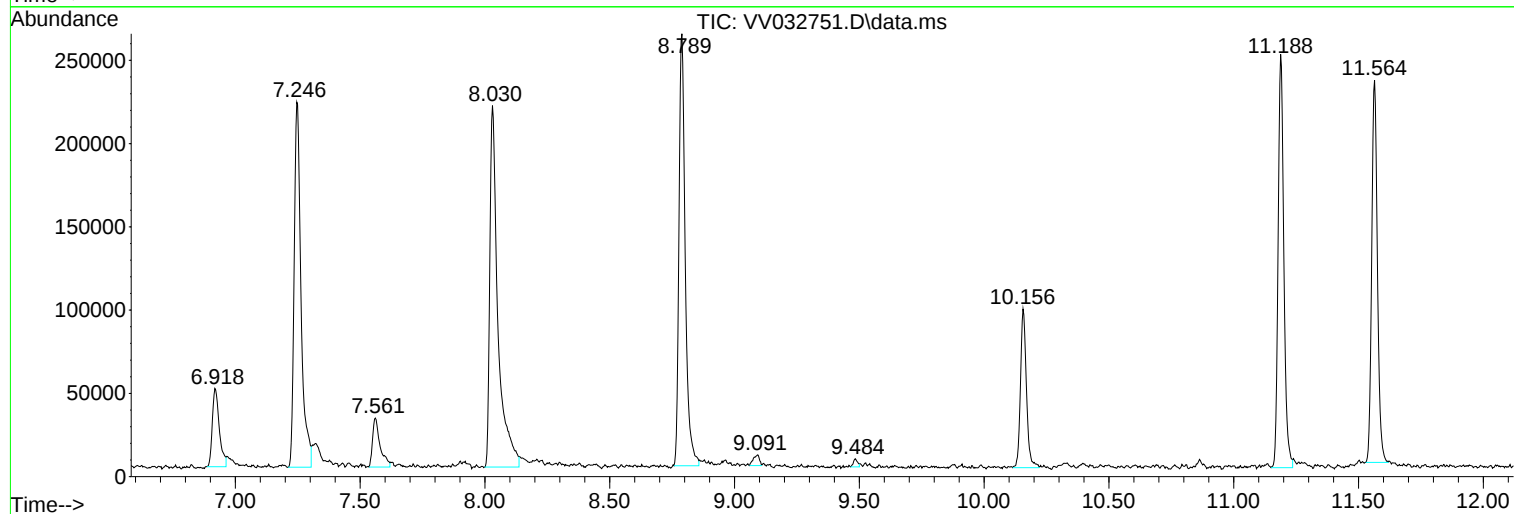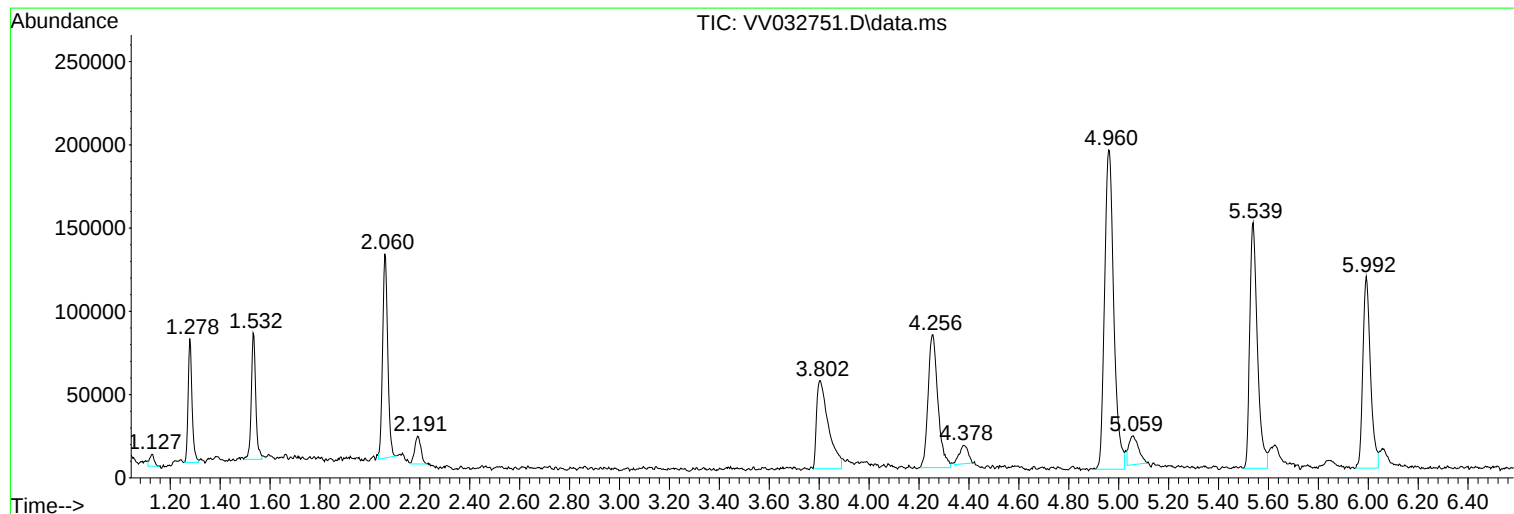

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032751.D
Acq On : 28 Oct 2023 18:56
Operator : SY/MD
Sample : 05103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032751.D
Acq On : 28 Oct 2023 18:56
Operator : SY/MD
Sample : 05103-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------