

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032752.D
 Acq On : 28 Oct 2023 19:21
 Operator : SY/MD
 Sample : 05103-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49X8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	22	27	35	rVB	8549	11830	2.38%	0.270%
2	1.278	67	74	86	rBV	74671	80587	16.24%	1.841%
3	1.532	146	153	169	rBV	77304	90614	18.26%	2.070%
4	2.060	307	317	328	rBV	122288	177764	35.81%	4.061%
5	2.188	351	357	371	rVB2	18159	34299	6.91%	0.784%
6	3.802	847	859	894	rBV2	58123	205333	41.37%	4.691%
7	4.253	984	999	1017	rBV	81636	215690	43.45%	4.927%
8	4.381	1029	1039	1054	rVB3	12381	27614	5.56%	0.631%
9	4.960	1200	1219	1240	rBV3	194059	496378	100.00%	11.340%
10	5.050	1240	1247	1260	rVB6	12688	33007	6.65%	0.754%
11	5.539	1385	1399	1416	rBV	147904	312971	63.05%	7.150%
12	5.613	1417	1422	1424	rBV5	5697	5871	1.18%	0.134%
13	5.992	1527	1540	1555	rBV2	112429	241566	48.67%	5.519%
14	6.918	1817	1828	1843	rBV	48558	99277	20.00%	2.268%
15	7.246	1918	1930	1951	rBV	217126	422707	85.16%	9.657%
16	7.561	2019	2028	2042	rBV2	29345	58202	11.73%	1.330%
17	8.031	2165	2174	2205	rBV	218431	492413	99.20%	11.249%
18	8.789	2399	2410	2435	rBV	252994	452249	91.11%	10.332%
19	10.156	2821	2835	2851	rBV	96439	161218	32.48%	3.683%
20	11.188	3146	3156	3172	rBV	247754	393574	79.29%	8.991%
21	11.564	3262	3273	3288	rBV	225791	364127	73.36%	8.319%




Sum of corrected areas: 4377291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032752.D
Acq On : 28 Oct 2023 19:21
Operator : SY/MD
Sample : 05103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

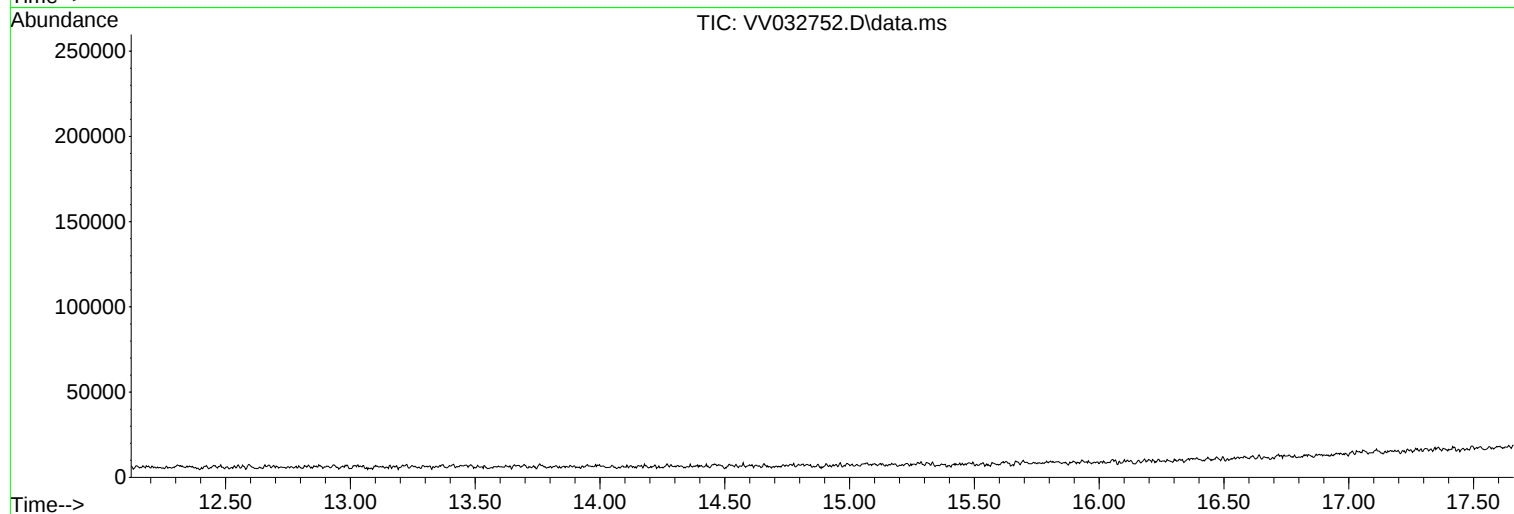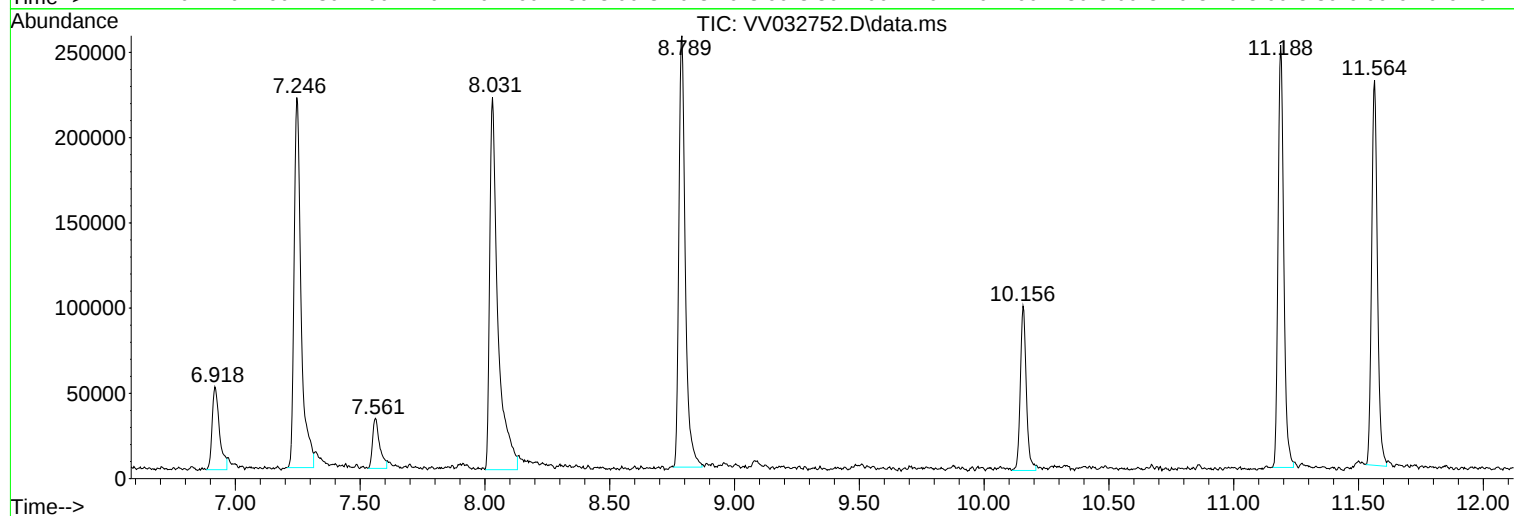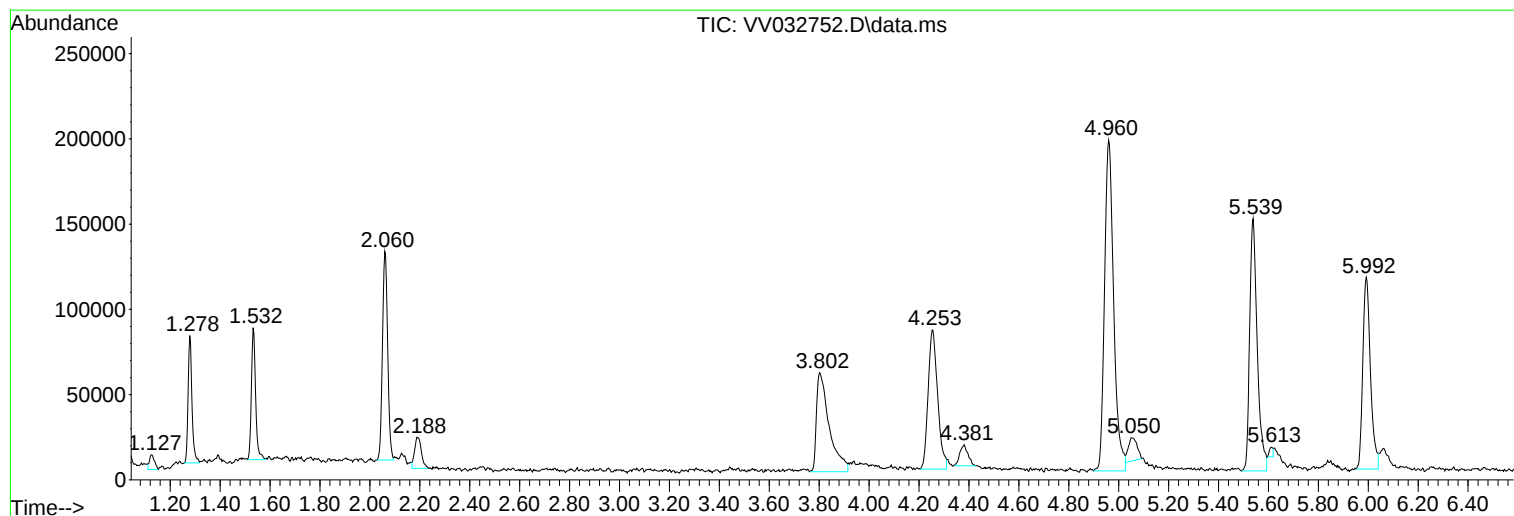

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032752.D
Acq On : 28 Oct 2023 19:21
Operator : SY/MD
Sample : 05103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032752.D
Acq On : 28 Oct 2023 19:21
Operator : SY/MD
Sample : 05103-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------