

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
 Data File : VV032753.D
 Acq On : 28 Oct 2023 19:45
 Operator : SY/MD
 Sample : 05103-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49Y0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	22	26	35	rVB	7871	9577	1.91%	0.215%
2	1.278	67	74	84	rBV	75075	80960	16.11%	1.821%
3	1.532	146	153	167	rVB	79304	93577	18.63%	2.105%
4	2.060	305	317	331	rBV	124111	184043	36.63%	4.140%
5	2.192	350	358	371	rVB2	18025	35100	6.99%	0.790%
6	3.802	848	859	881	rBV	52543	160604	31.97%	3.613%
7	4.253	983	999	1022	rBV2	83937	223785	44.54%	5.034%
8	4.378	1028	1038	1040	rBV3	10594	15963	3.18%	0.359%
9	4.960	1202	1219	1239	rBV2	196345	501098	99.74%	11.273%
10	5.063	1242	1251	1269	rVB3	18244	51014	10.15%	1.148%
11	5.539	1386	1399	1415	rBV	151413	322257	64.14%	7.249%
12	5.992	1526	1540	1555	rBV	116160	248128	49.39%	5.582%
13	6.918	1820	1828	1840	rBV	48502	89175	17.75%	2.006%
14	7.246	1920	1930	1951	rBV	222843	428144	85.22%	9.632%
15	7.561	2019	2028	2050	rBV	30403	63231	12.59%	1.422%
16	8.031	2165	2174	2217	rBV	218148	502408	100.00%	11.302%
17	8.789	2398	2410	2436	rBV	263684	473944	94.33%	10.662%
18	9.075	2488	2499	2501	rBV	4775	6481	1.29%	0.146%
19	10.156	2822	2835	2851	rBV2	94966	160657	31.98%	3.614%
20	11.188	3145	3156	3176	rBV	254167	414357	82.47%	9.321%
21	11.500	3245	3253	3257	rBV9	4800	6671	1.33%	0.150%
22	11.564	3262	3273	3291	rVB	226618	374064	74.45%	8.415%




Sum of corrected areas: 4445238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032753.D
Acq On : 28 Oct 2023 19:45
Operator : SY/MD
Sample : 05103-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

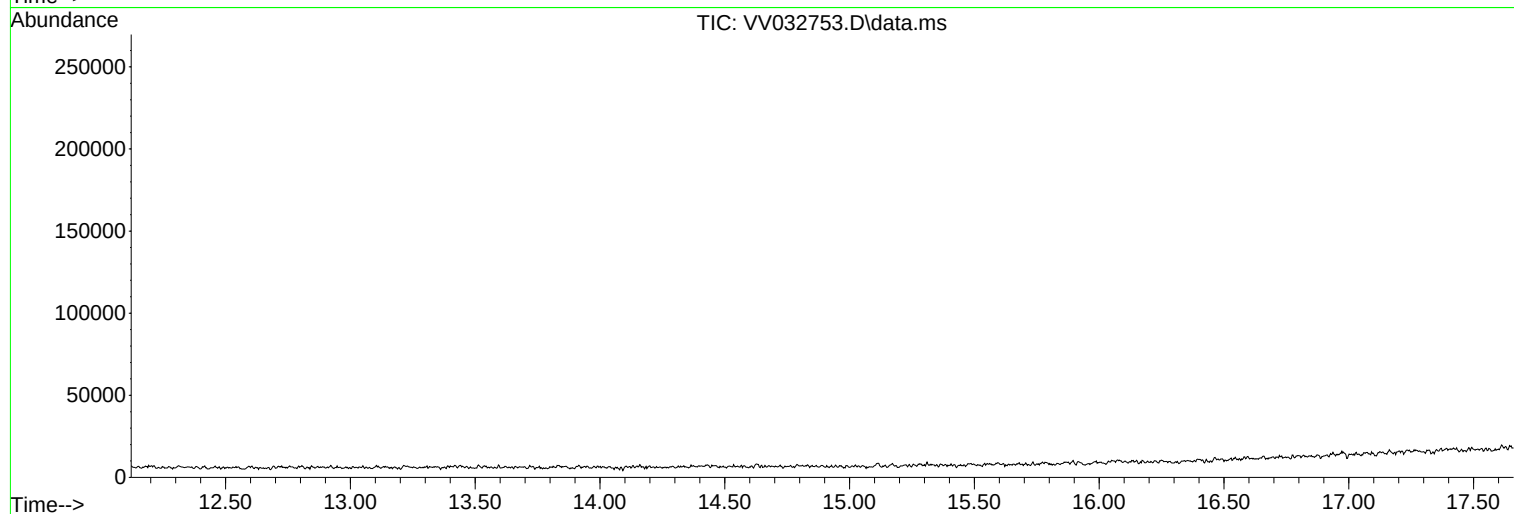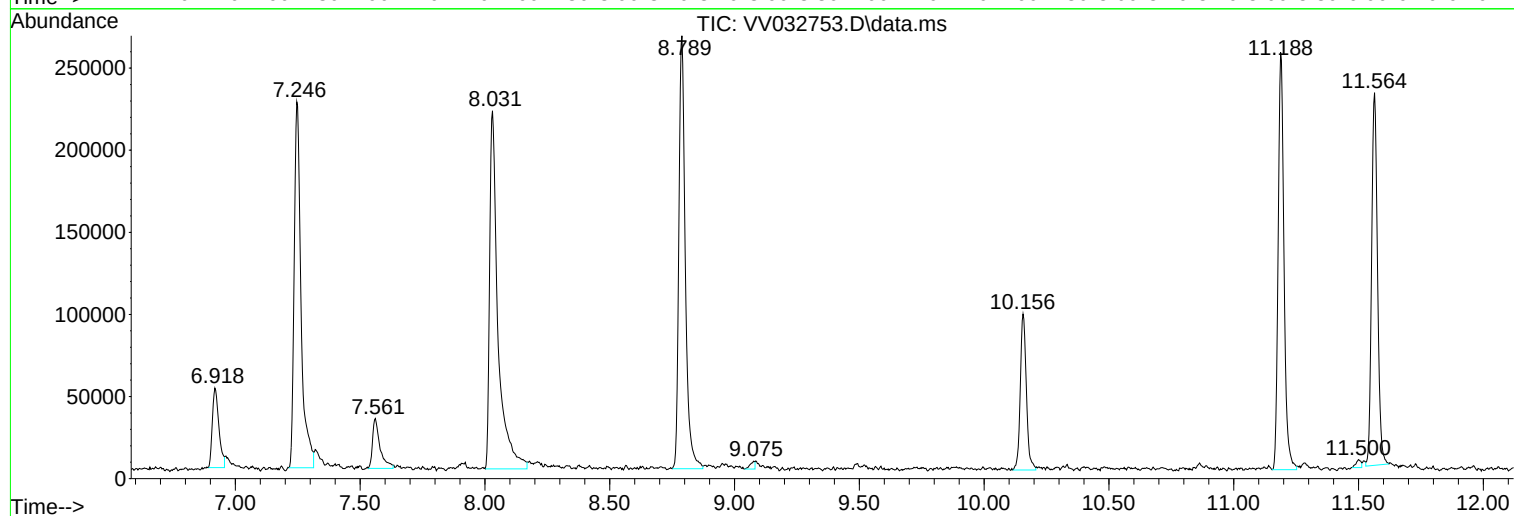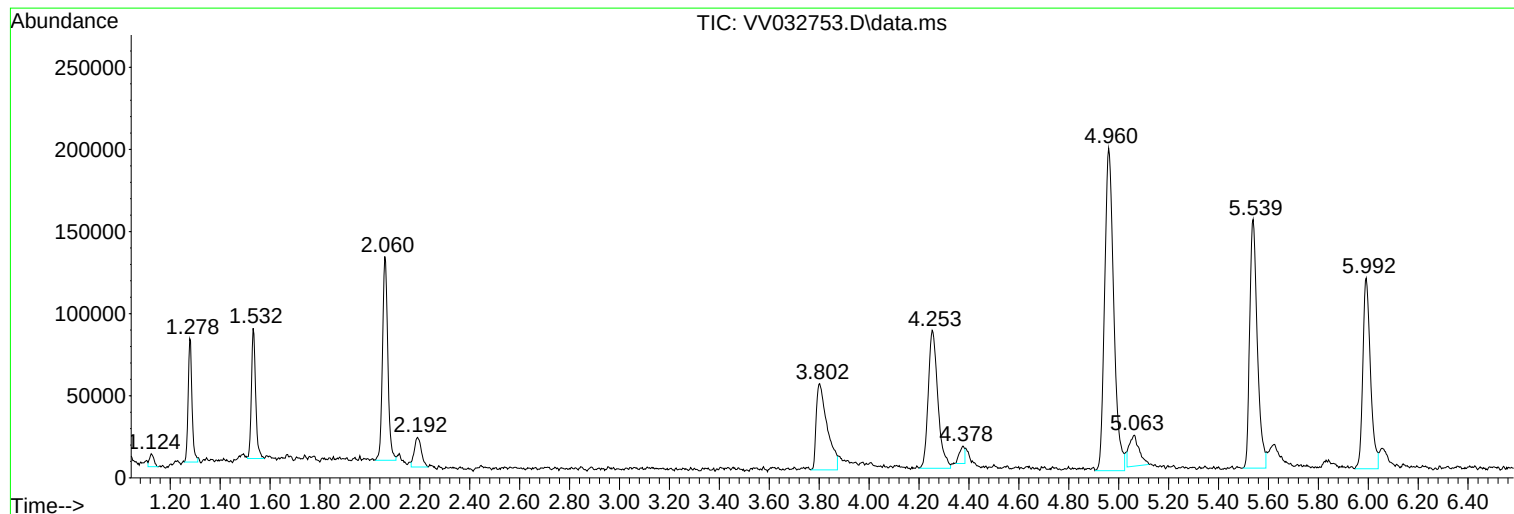

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032753.D
Acq On : 28 Oct 2023 19:45
Operator : SY/MD
Sample : 05103-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032753.D
Acq On : 28 Oct 2023 19:45
Operator : SY/MD
Sample : 05103-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------