
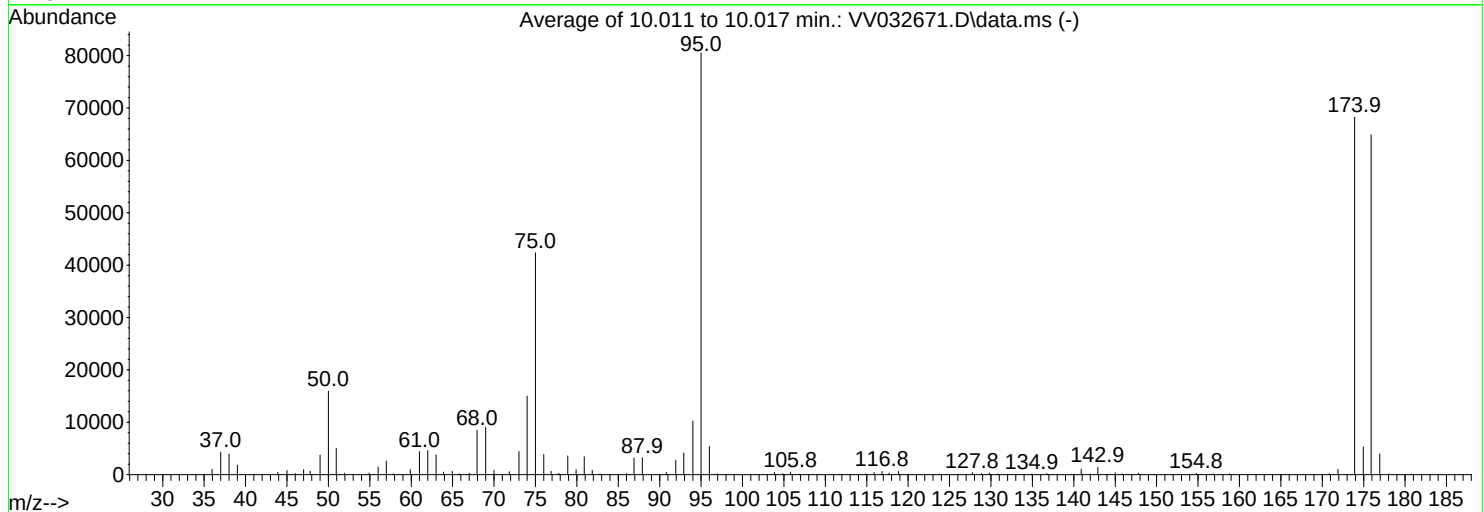


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102723\
Data File : VV032671.D
Acq On : 27 Oct 2023 08:30
Operator : SY/MD
Sample : BFB229
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB229

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Oct 31 02:23:31 2023

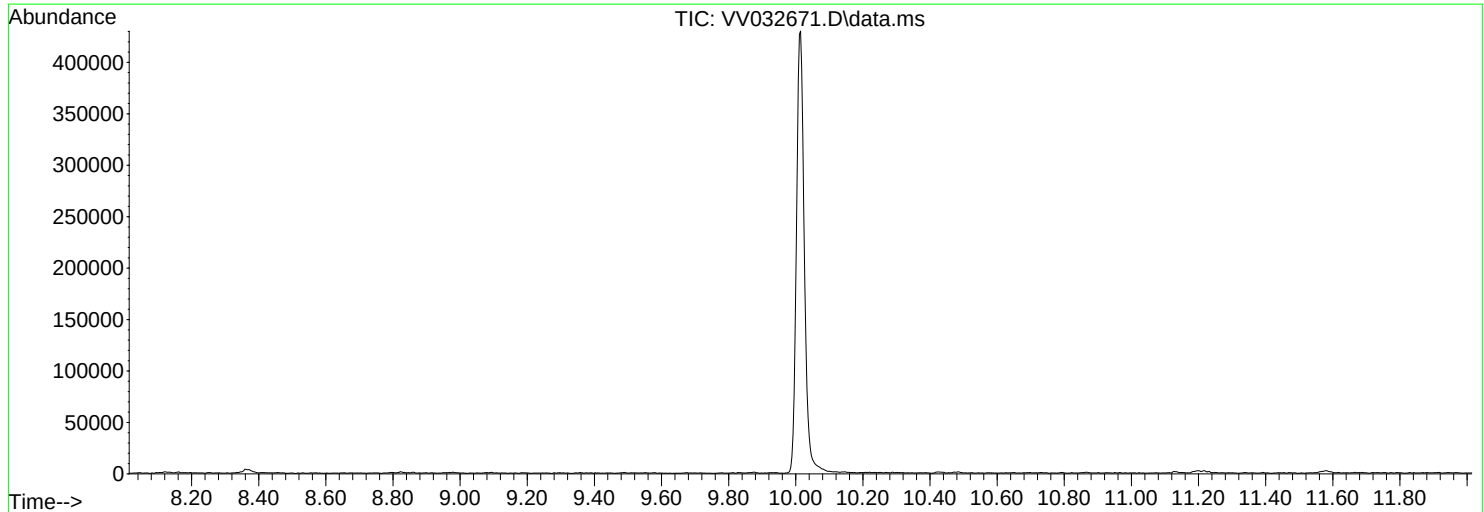

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	15962	PASS
75	95	30	80	52.6	42371	PASS
95	95	100	100	100.0	80528	PASS
96	95	5	9	6.7	5394	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	68243	PASS
175	174	5	9	7.8	5291	PASS
176	174	95	105	95.1	64883	PASS
177	176	5	10	6.1	3972	PASS

m/z	Abundance
35.60	125.0
39.80	213.0
40.80	117.0
41.10	115.0
43.90	297.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
36.00	1033.0
37.00	4456.0
38.00	4062.0
39.00	1907.0
39.90	229.0
42.90	102.0
44.00	759.0
45.00	843.0
46.00	220.0
47.00	959.0
47.80	647.0
49.00	3938.0
50.00	16696.0
51.00	5171.0
51.90	305.0
53.00	144.0
53.60	116.0
54.90	293.0
56.00	1449.0
57.00	2624.0
57.90	140.0
59.90	1107.0
61.00	4474.0
62.00	4742.0
63.00	3966.0
63.90	553.0
65.00	697.0
65.90	140.0
67.00	301.0
67.90	8775.0
69.00	9296.0
70.00	809.0
70.90	104.0
71.80	564.0
73.00	4587.0
74.00	15460.0
75.00	44248.0
76.00	3913.0
76.90	668.0
77.70	326.0
78.90	3688.0
79.90	906.0
80.90	3594.0
81.90	885.0
82.80	159.0
86.00	195.0
86.90	3374.0
87.90	3316.0
90.80	506.0
92.00	2803.0
92.90	4178.0
94.00	10630.0
95.00	82680.0
96.00	5647.0
97.00	218.0
103.80	466.0
104.90	173.0
105.80	498.0
110.90	165.0
111.70	112.0
112.70	101.0
114.90	156.0
115.90	457.0
116.80	637.0
117.70	311.0
118.90	621.0
127.80	407.0
128.80	231.0
129.80	266.0
130.90	156.0
134.90	148.0
136.80	252.0
140.00	103.0
140.90	1149.0
141.90	153.0
142.90	1420.0
145.00	436.0
145.80	184.0
147.80	280.0
149.70	153.0
154.80	234.0
156.80	182.0
158.80	148.0
170.90	213.0
171.90	1063.0
173.90	67864.0
174.90	5510.0
175.90	65032.0
177.00	4189.0
178.00	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
35.90	1024.0
37.00	4406.0
38.00	4084.0
39.00	1846.0
39.90	240.0
44.00	731.0
45.00	832.0
46.00	240.0
47.00	990.0
47.80	681.0
49.00	3828.0
50.00	16383.0
51.00	5185.0
51.90	278.0
53.00	120.0
54.90	319.0
56.00	1437.0
57.00	2670.0
57.80	156.0
59.90	967.0
61.00	4514.0
62.00	4769.0
63.00	3926.0
63.90	517.0
65.00	661.0
65.90	156.0
67.00	276.0
67.90	8638.0
69.00	9421.0
70.00	847.0
71.90	575.0
73.00	4656.0
74.00	15493.0
75.00	43760.0
76.00	3923.0
76.90	623.0
77.90	352.0
78.90	3691.0
79.90	959.0
80.90	3516.0
81.90	851.0
82.80	168.0
86.00	205.0
86.90	3225.0
87.90	3356.0
90.80	452.0
92.00	2806.0
92.90	4309.0
94.00	10486.0
95.00	83064.0
96.00	5523.0
97.00	203.0
103.90	466.0
104.80	188.0
105.80	524.0
106.90	111.0
110.90	140.0
111.90	124.0
112.70	103.0
114.90	145.0
115.90	419.0
116.80	633.0
117.70	323.0
118.90	628.0
127.70	426.0
128.80	216.0
129.80	291.0
130.90	129.0
135.00	168.0
136.80	253.0
140.00	106.0
140.90	1097.0
141.90	156.0
142.90	1470.0
143.90	116.0
145.00	398.0
145.90	133.0
147.80	286.0
149.70	132.0
154.80	274.0
156.90	162.0
158.80	165.0
170.80	186.0
171.90	1039.0
173.90	70400.0
174.90	5513.0
175.90	66976.0
177.00	4072.0
178.00	178.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229

m/z	Abundance
35.90	944.0
37.00	3950.0
38.00	3727.0
39.00	1642.0
39.90	232.0
40.70	109.0
43.90	727.0
45.00	728.0
46.00	224.0
47.00	914.0
47.80	576.0
49.00	3411.0
50.00	14808.0
50.90	4791.0
52.00	226.0
54.90	299.0
56.00	1406.0
57.00	2458.0
57.80	158.0
59.90	824.0
61.00	4138.0
62.00	4315.0
63.00	3511.0
63.90	440.0
64.90	599.0
65.80	148.0
67.10	243.0
68.00	7991.0
69.00	8557.0
70.00	802.0
71.90	474.0
73.00	4021.0
74.00	14038.0
75.00	39104.0
76.00	3624.0
76.90	594.0
77.80	341.0
78.90	3374.0
79.90	969.0
80.90	3155.0
81.80	756.0
82.80	160.0
86.00	201.0
86.90	2900.0
87.90	3058.0
90.80	353.0
91.90	2640.0
92.90	3948.0
94.00	9560.0
95.00	75840.0
96.00	5012.0
96.90	165.0
103.90	436.0
104.80	169.0
105.80	457.0
106.90	131.0
110.60	104.0
111.00	105.0
112.00	128.0
114.90	129.0
115.90	377.0
116.90	588.0
117.70	301.0
118.80	565.0
127.70	380.0
128.90	169.0
129.80	322.0
130.80	105.0
135.00	178.0
136.70	214.0
140.90	932.0
142.00	125.0
142.90	1365.0
143.80	116.0
144.90	267.0
145.80	103.0
147.80	264.0
152.80	106.0
154.80	250.0
155.80	115.0
156.90	117.0
158.80	143.0
170.80	160.0
171.90	923.0
173.90	66464.0
175.00	4849.0
175.90	62640.0
176.90	3656.0
178.10	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB229