


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102820\
 Data File : VV019131.D
 Acq On : 28 Oct 2020 09:21
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 29 03:08:29 2020

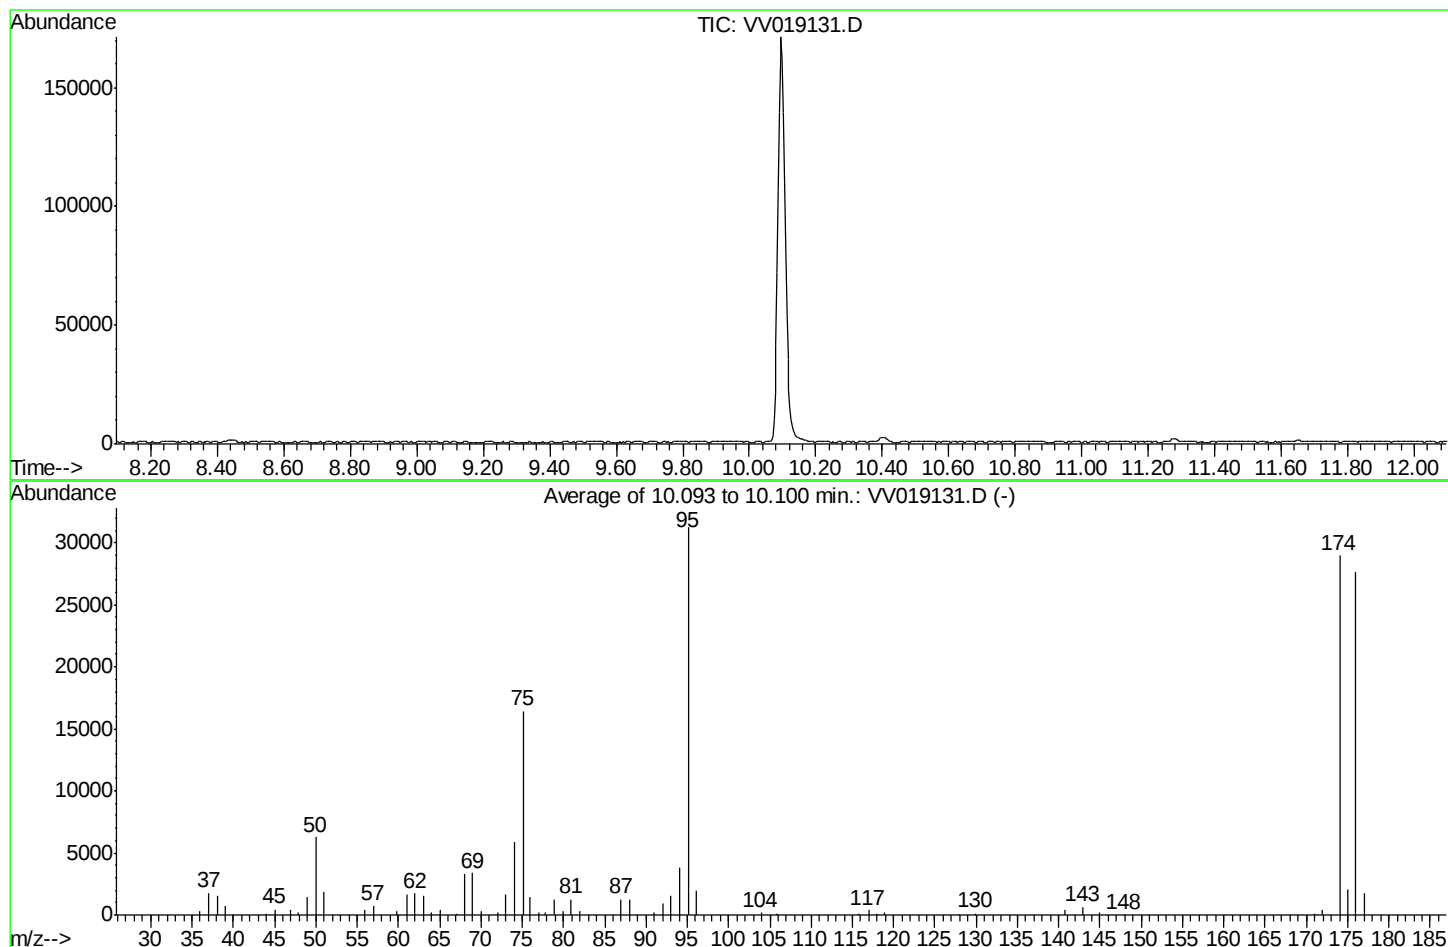

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	6260	PASS
75	95	30	80	52.7	16449	PASS
95	95	100	100	100.0	31240	PASS
96	95	5	9	6.3	1974	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.7	28973	PASS
175	174	5	9	7.0	2041	PASS
176	174	95	101	95.4	27632	PASS
177	176	5	9	6.5	1800	PASS

m/z	Abundance
35.90	362.0
37.00	1797.0
38.10	1564.0
39.00	686.0
40.00	181.0
44.00	907.0
45.00	474.0
47.00	402.0
47.90	190.0
49.00	1454.0
50.00	6137.0
51.00	1831.0
56.00	477.0
57.00	795.0
59.90	347.0
61.00	1616.0
62.00	1717.0
63.10	1518.0
63.90	264.0
65.10	403.0
67.00	116.0
68.00	3344.0
69.00	3416.0
70.00	286.0
72.00	190.0
73.00	1634.0
74.00	5722.0
75.10	16472.0
76.00	1476.0
77.00	216.0
77.90	220.0
78.90	1254.0
80.00	363.0
80.90	1219.0
81.90	327.0
87.00	1280.0
88.00	1236.0
91.10	172.0
92.00	1033.0
93.00	1609.0
94.00	3818.0
95.10	31016.0
96.10	2083.0
104.00	171.0
105.90	120.0
115.80	104.0
117.00	348.0
117.90	168.0
119.00	255.0
130.00	134.0
140.80	395.0
143.00	617.0
144.90	174.0
147.90	111.0
171.00	119.0
171.90	372.0
174.00	27944.0
175.10	2110.0
176.00	26600.0
177.00	1843.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	348.0
37.10	1830.0
38.00	1651.0
39.00	749.0
40.10	189.0
44.00	977.0
45.10	435.0
47.00	441.0
47.80	205.0
49.00	1489.0
50.00	6462.0
51.00	1866.0
56.00	469.0
57.00	734.0
59.90	373.0
61.00	1757.0
62.00	1775.0
63.10	1583.0
64.00	278.0
65.00	460.0
67.10	106.0
68.00	3391.0
69.00	3449.0
70.00	372.0
72.00	253.0
73.00	1693.0
74.10	6032.0
75.10	17000.0
76.00	1466.0
77.00	230.0
77.90	200.0
78.90	1297.0
80.00	361.0
80.90	1311.0
81.90	328.0
87.00	1333.0
87.90	1244.0
91.00	164.0
92.00	971.0
93.00	1640.0
94.00	3929.0
95.10	32504.0
96.10	2053.0
103.90	168.0
105.90	142.0
115.80	125.0
117.00	360.0
117.90	152.0
118.90	253.0
129.90	148.0
140.80	416.0
142.90	669.0
145.00	169.0
171.00	133.0
171.90	444.0
174.00	30264.0
175.00	2067.0
176.00	28568.0
177.00	1851.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.90	275.0
37.10	1697.0
38.00	1581.0
39.00	692.0
40.10	171.0
44.00	993.0
45.00	374.0
47.00	433.0
47.80	197.0
49.00	1385.0
50.00	6182.0
51.00	1805.0
56.00	445.0
57.00	756.0
59.80	349.0
61.00	1735.0
62.00	1647.0
63.00	1511.0
64.00	240.0
65.00	459.0
68.00	3233.0
69.00	3223.0
70.00	374.0
72.10	274.0
73.00	1581.0
74.10	5815.0
75.10	15876.0
76.00	1349.0
77.00	234.0
77.80	166.0
78.90	1134.0
80.00	355.0
80.90	1286.0
81.90	298.0
87.00	1200.0
87.90	1137.0
90.90	144.0
92.00	928.0
93.00	1514.0
94.00	3693.0
95.10	30200.0
96.10	1786.0
103.90	156.0
105.90	160.0
115.80	139.0
116.90	393.0
117.90	114.0
118.80	230.0
127.80	115.0
129.90	149.0
140.80	384.0
142.90	619.0
145.10	194.0
171.00	118.0
172.00	477.0
174.00	28712.0
175.00	1948.0
176.00	27728.0
176.90	1708.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

Scan 2790 (10.061 min): VV019131.D
BFB84

m/z	Abundance
39.90	140.0
44.00	812.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84