

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023082.D
 Acq On : 28 Oct 2021 18:30
 Operator : SY/MD
 Sample : VV1028MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 29 02:15:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 29 01:52:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	291776	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	281098	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	135780	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	93039	46.269	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.540%
7) Chloroethane-d5	1.568	69	72764	46.394	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.780%
11) 1,1-Dichloroethene-d2	2.108	63	132900	34.891	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.780%
21) 2-Butanone-d5	3.879	46	157578	104.596	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.600%
24) Chloroform-d	4.349	84	194658	46.042	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.080%
26) 1,2-Dichloroethane-d4	5.034	65	123610	49.396	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.800%
32) Benzene-d6	5.053	84	385646	50.082	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.160%
36) 1,2-Dichloropropane-d6	6.069	67	122517	49.981	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.960%
41) Toluene-d8	7.317	98	338817	48.228	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.460%
43) trans-1,3-Dichloroprop...	7.622	79	55440	47.187	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.380%
47) 2-Hexanone-d5	8.088	63	117717	110.566	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.570%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	174097	48.593	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.180%
66) 1,2-Dichlorobenzene-d4	11.625	152	139581	53.293	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.580%
Target Compounds						
72) 1,2,3-Trichlorobenzene	13.747	180	1480	0.487	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023082.D
Acq On : 28 Oct 2021 18:30
Operator : SY/MD
Sample : VV1028MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 29 02:15:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 29 01:52:27 2021
Response via : Initial Calibration

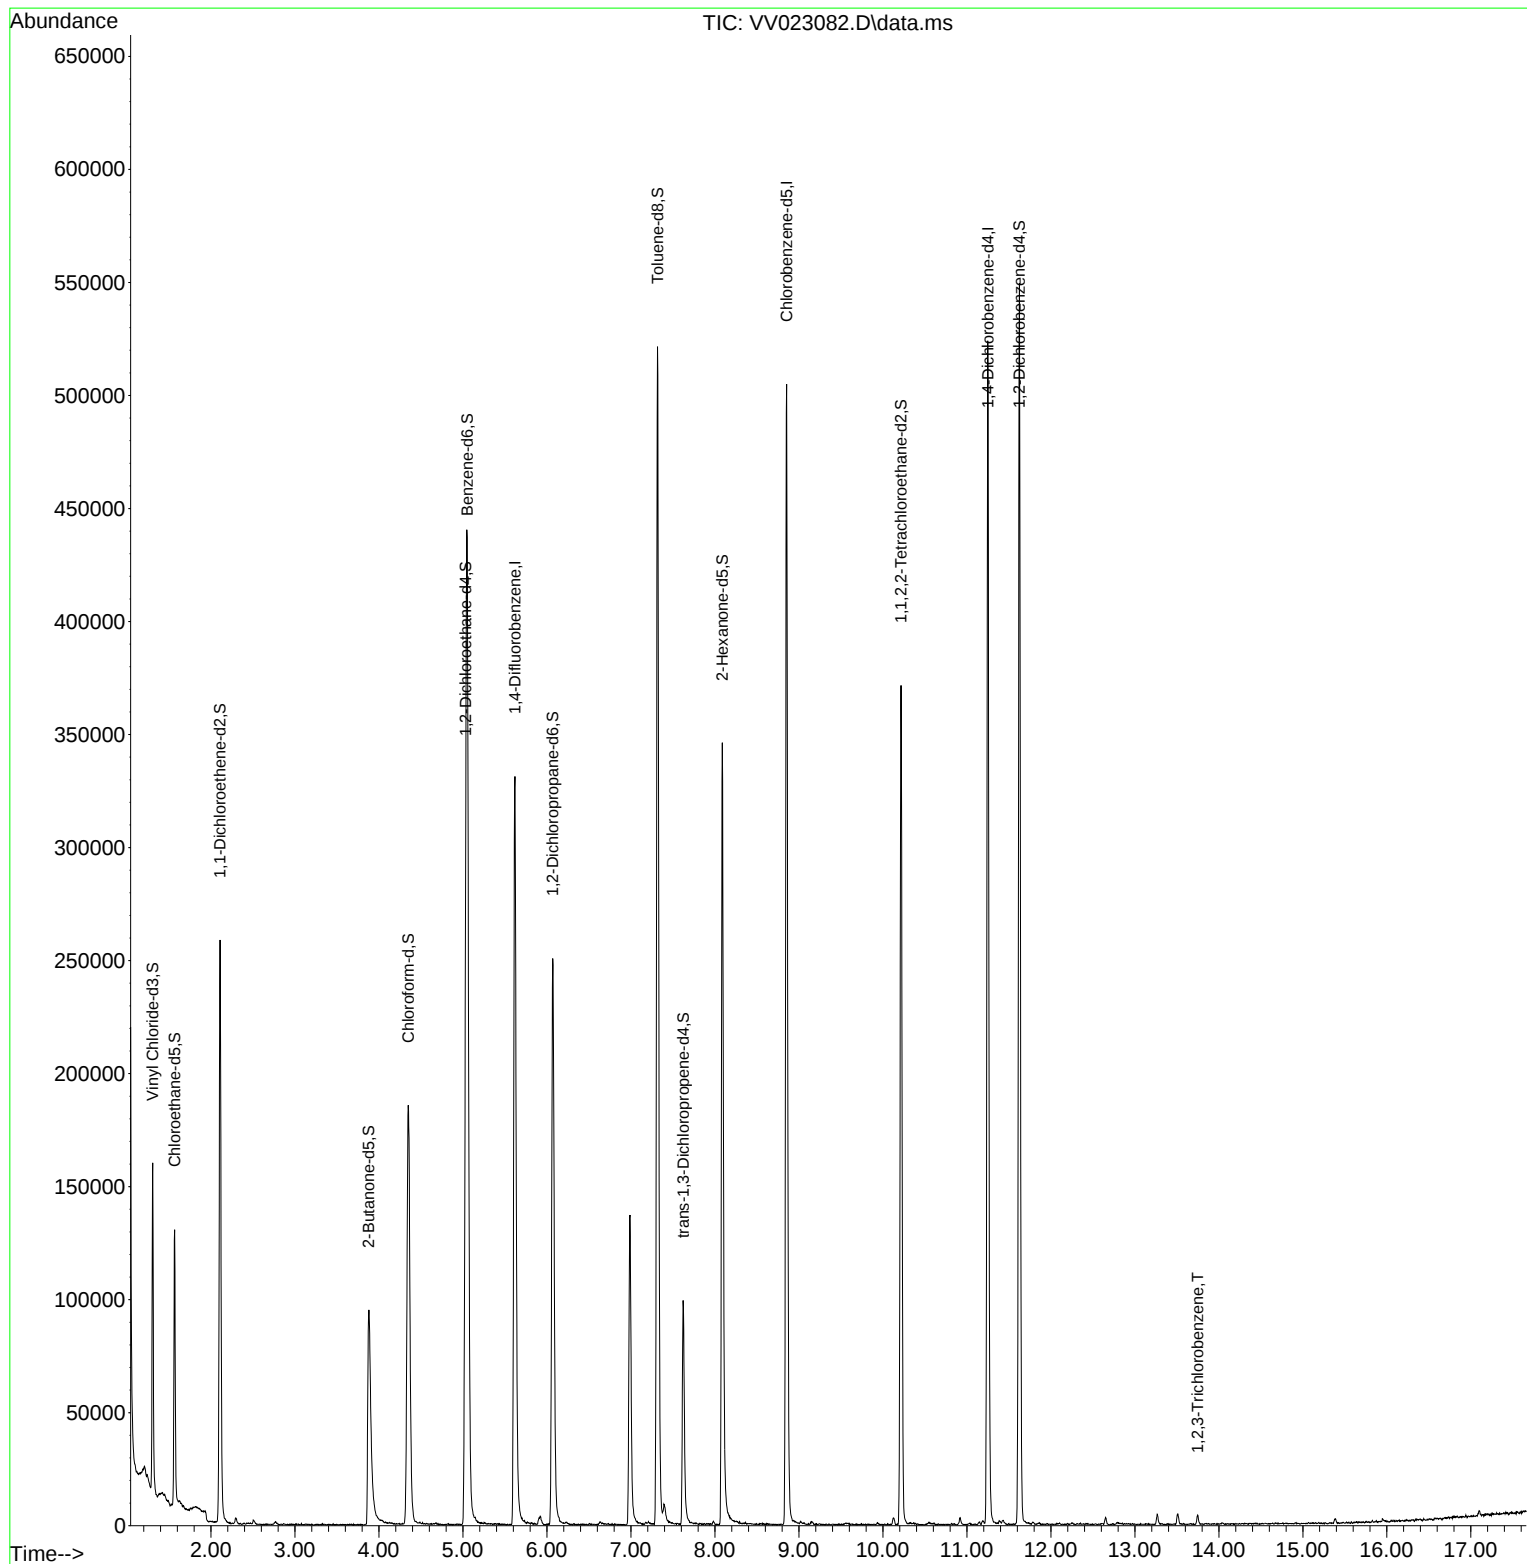

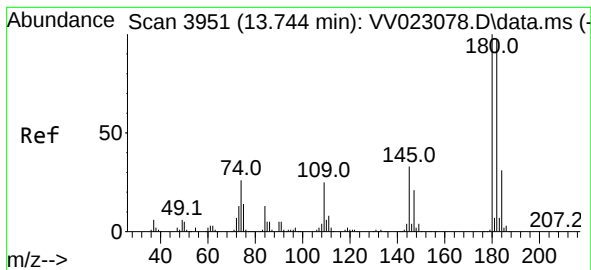

#72
 1,2,3-Trichlorobenzene
 Concen: 0.487 ug/L
 RT: 13.747 min Scan# 3952
 Delta R.T. 0.003 min
 Lab File: VV023082.D
 Acq: 28 Oct 2021 18:30

Instrument :
 MSVOA_V
 ClientSampleId :

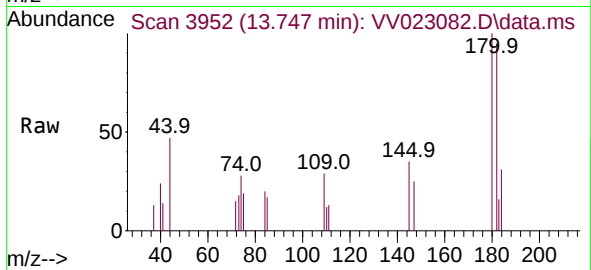

Tgt Ion:	180	Resp:	1480
Ion	Ratio	Lower	Upper
180	100		
182	83.5	77.0	115.4
145	26.4	26.4	39.6

