

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023082.D
 Acq On : 28 Oct 2021 18:30
 Operator : SY/MD
 Sample : VV1028MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

Signal : TIC: VV023082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	146716	152397	13.40%	1.747%
2	1.568	158	164	178	rVB	120415	131843	11.59%	1.512%
3	2.108	322	332	360	rVB	257580	382632	33.65%	4.387%
4	2.503	451	455	468	rVB5	1915	2808	0.25%	0.032%
5	2.953	591	595	599	rBV	457	379	0.03%	0.004%
6	3.198	667	671	677	rVB2	405	351	0.03%	0.004%
7	3.455	747	751	754	rBV3	456	282	0.02%	0.003%
8	3.494	761	763	768	rBV	294	271	0.02%	0.003%
9	3.773	845	850	853	rBV2	307	238	0.02%	0.003%
10	3.844	864	872	873	rBV	317	310	0.03%	0.004%
11	3.879	873	883	911	rBV	94897	256675	22.57%	2.943%
12	4.349	1013	1029	1055	rBV	185170	462205	40.64%	5.300%
13	4.703	1137	1139	1142	rVB	660	324	0.03%	0.004%
14	4.812	1170	1173	1176	rBV4	323	251	0.02%	0.003%
15	4.892	1193	1198	1199	rBV2	364	269	0.02%	0.003%
16	4.928	1207	1209	1215	rVB2	437	361	0.03%	0.004%
17	4.953	1215	1217	1219	rBV	340	214	0.02%	0.002%
18	5.047	1229	1246	1274	rBV2	439861	1137218	100.00%	13.039%
19	5.252	1308	1310	1311	rBV	593	232	0.02%	0.003%
20	5.365	1342	1345	1346	rBV	357	231	0.02%	0.003%
21	5.529	1393	1396	1401	rVB3	363	234	0.02%	0.003%
22	5.551	1401	1403	1406	rBV2	325	210	0.02%	0.002%
23	5.619	1410	1424	1449	rBV	330954	669132	58.84%	7.672%
24	5.908	1506	1514	1515	rBV3	3078	3141	0.28%	0.036%
25	5.992	1537	1540	1543	rBV3	317	231	0.02%	0.003%
26	6.069	1551	1564	1586	rBV	250265	514134	45.21%	5.895%
27	6.297	1631	1635	1637	rVB2	311	218	0.02%	0.002%
28	6.320	1637	1642	1645	rBV3	532	463	0.04%	0.005%
29	6.371	1654	1658	1661	rBV3	448	384	0.03%	0.004%
30	6.403	1666	1668	1673	rVB	349	253	0.02%	0.003%
31	6.426	1673	1675	1680	rVB3	448	389	0.03%	0.004%
32	6.506	1695	1700	1703	rBV2	623	571	0.05%	0.007%
33	6.635	1733	1740	1746	rBV6	1237	1954	0.17%	0.022%
34	6.780	1782	1785	1788	rVB2	463	216	0.02%	0.002%
35	6.805	1788	1793	1796	rBV2	558	448	0.04%	0.005%
36	6.857	1805	1809	1812	rBV	382	275	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023082.D
 Acq On : 28 Oct 2021 18:30
 Operator : SY/MD
 Sample : VV1028MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.989	1834	1850	1874	rBV	137139	253268	22.27%	2.904%
38	7.317	1940	1952	1970	rBV	520969	896816	78.86%	10.283%
39	7.555	2022	2026	2027	rBV2	487	372	0.03%	0.004%
40	7.622	2037	2047	2072	rBV	99112	173447	15.25%	1.989%
41	7.815	2105	2107	2109	rBV	456	266	0.02%	0.003%
42	7.902	2130	2134	2138	rBV2	489	485	0.04%	0.006%
43	7.950	2146	2149	2154	rBV3	510	447	0.04%	0.005%
44	7.982	2154	2159	2169	rVB6	1658	2323	0.20%	0.027%
45	8.024	2169	2172	2173	rBV	458	251	0.02%	0.003%
46	8.053	2178	2181	2182	rBV2	504	285	0.03%	0.003%
47	8.088	2182	2192	2221	rBV	345655	576839	50.72%	6.614%
48	8.294	2254	2256	2260	rVB3	899	449	0.04%	0.005%
49	8.780	2403	2407	2409	rBV3	260	209	0.02%	0.002%
50	8.854	2418	2430	2452	rBV	504282	817661	71.90%	9.375%
51	9.140	2516	2519	2520	rBV2	789	377	0.03%	0.004%
52	9.210	2539	2541	2544	rVB2	461	211	0.02%	0.002%
53	9.323	2573	2576	2581	rBV2	427	351	0.03%	0.004%
54	9.358	2583	2587	2595	rBV2	447	473	0.04%	0.005%
55	9.477	2622	2624	2628	rVB2	440	299	0.03%	0.003%
56	9.506	2628	2633	2635	rBV2	490	357	0.03%	0.004%
57	9.616	2665	2667	2670	rBV	414	356	0.03%	0.004%
58	9.744	2705	2707	2713	rVB2	627	402	0.04%	0.005%
59	9.773	2713	2716	2718	rBV3	312	223	0.02%	0.003%
60	9.821	2727	2731	2735	rBV3	383	339	0.03%	0.004%
61	9.937	2761	2767	2769	rVV5	973	841	0.07%	0.010%
62	10.021	2788	2793	2798	rBV3	370	372	0.03%	0.004%
63	10.056	2801	2804	2806	rBV2	509	283	0.02%	0.003%
64	10.124	2820	2825	2834	rVB5	3052	4700	0.41%	0.054%
65	10.217	2842	2854	2877	rBV	371236	585057	51.45%	6.708%
66	10.381	2903	2905	2910	rVB3	606	461	0.04%	0.005%
67	10.509	2940	2945	2946	rBV	275	203	0.02%	0.002%
68	10.609	2973	2976	2978	rBV3	563	306	0.03%	0.004%
69	10.661	2988	2992	2995	rBV4	481	403	0.04%	0.005%
70	10.741	3014	3017	3022	rBV2	287	330	0.03%	0.004%
71	10.818	3039	3041	3045	rVB3	520	308	0.03%	0.004%
72	10.847	3047	3050	3060	rVB3	482	462	0.04%	0.005%
73	10.921	3063	3073	3081	rVB6	3059	4616	0.41%	0.053%
74	11.152	3135	3145	3150	rBV4	1280	1914	0.17%	0.022%
75	11.188	3150	3156	3157	rBV3	1606	1486	0.13%	0.017%
76	11.249	3164	3175	3197	rBV	523056	791983	69.64%	9.081%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023082.D
 Acq On : 28 Oct 2021 18:30
 Operator : SY/MD
 Sample : VV1028MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

77	11.384	3214	3217	3219	rBV4	1180	881	0.08%	0.010%
78	11.500	3247	3253	3256	rBV4	635	476	0.04%	0.005%
79	11.551	3266	3269	3273	rBV2	411	247	0.02%	0.003%
80	11.625	3280	3292	3311	rBV	548348	843548	74.18%	9.672%
81	11.783	3335	3341	3350	rVB6	991	1644	0.14%	0.019%
82	11.953	3390	3394	3396	rBV2	531	379	0.03%	0.004%
83	11.976	3399	3401	3407	rVB3	247	202	0.02%	0.002%
84	12.072	3426	3431	3434	rBV3	616	465	0.04%	0.005%
85	12.564	3581	3584	3587	rBV	366	265	0.02%	0.003%
86	12.596	3591	3594	3595	rBV2	338	203	0.02%	0.002%
87	12.651	3604	3611	3625	rVB6	3320	5052	0.44%	0.058%
88	12.709	3625	3629	3632	rBV2	287	243	0.02%	0.003%
89	12.763	3643	3646	3648	rBV3	355	287	0.03%	0.003%
90	12.972	3708	3711	3714	rVB2	403	243	0.02%	0.003%
91	13.265	3794	3802	3814	rBV6	4564	6953	0.61%	0.080%
92	13.384	3836	3839	3842	rBV	492	299	0.03%	0.003%
93	13.509	3870	3878	3887	rBV2	4708	7511	0.66%	0.086%
94	13.747	3944	3952	3961	rVB5	4075	5672	0.50%	0.065%
95	13.837	3976	3980	3984	rBV3	492	593	0.05%	0.007%
96	14.098	4058	4061	4062	rBV2	358	207	0.02%	0.002%
97	14.149	4073	4077	4080	rBV2	406	400	0.04%	0.005%
98	14.368	4141	4145	4147	rBV2	465	443	0.04%	0.005%
99	14.705	4247	4250	4251	rBV	493	214	0.02%	0.002%
100	15.387	4455	4462	4469	rVB9	2115	3107	0.27%	0.036%




Sum of corrected areas: 8721509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023082.D
Acq On : 28 Oct 2021 18:30
Operator : SY/MD
Sample : VV1028MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

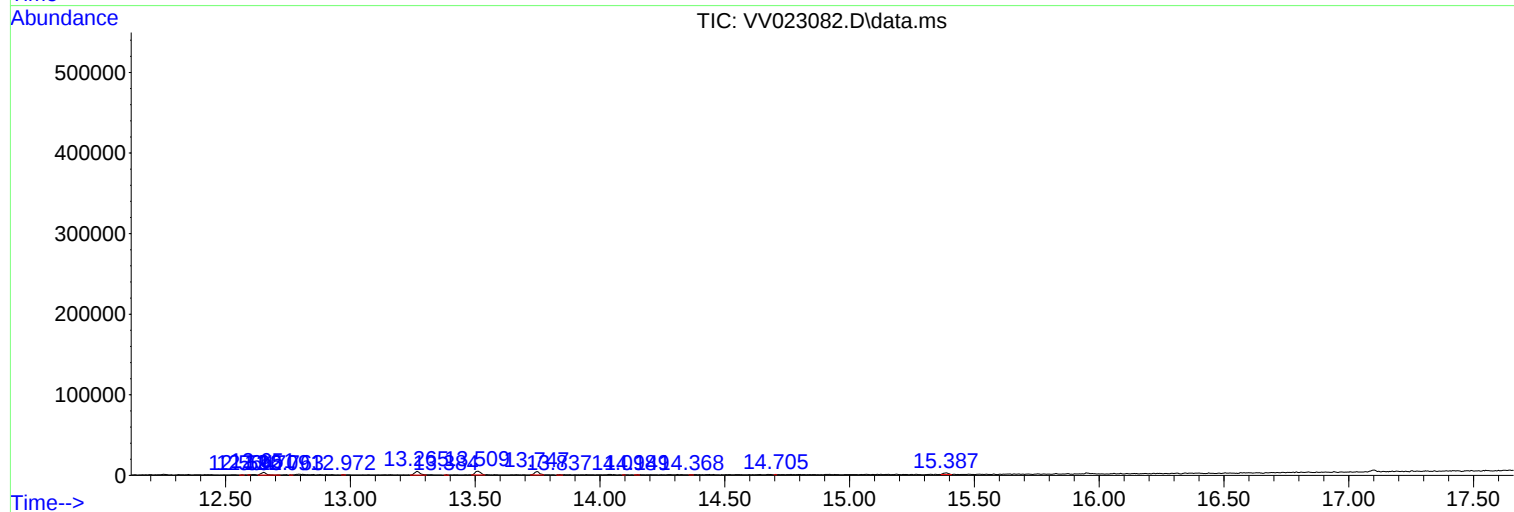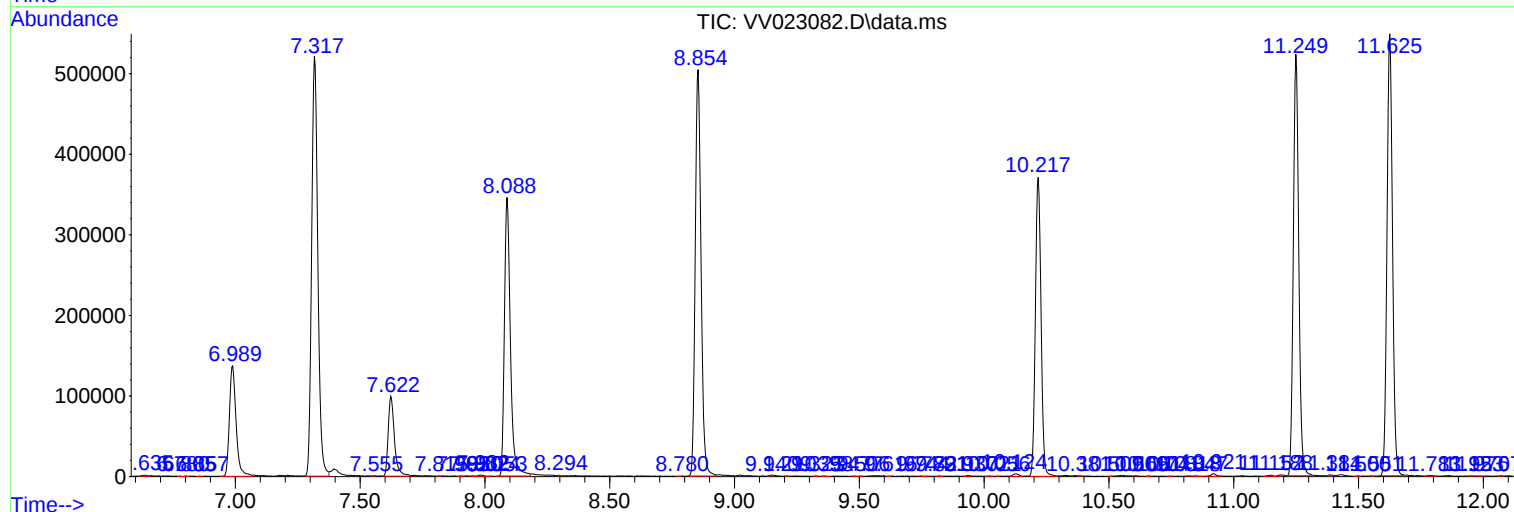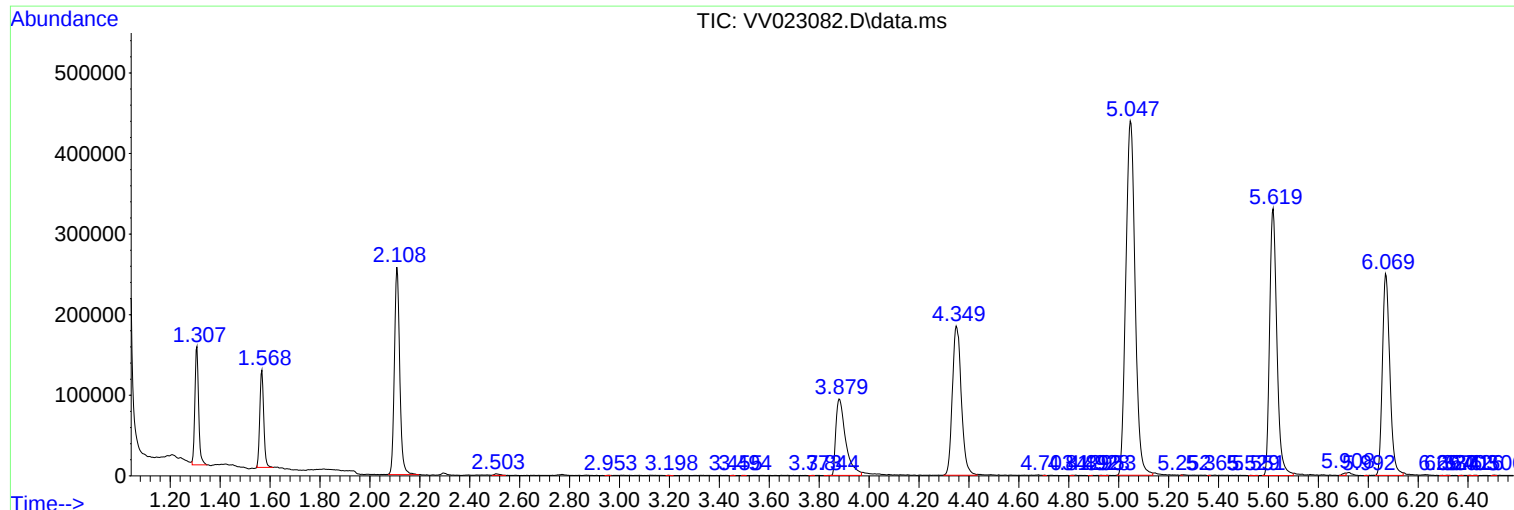

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023082.D
Acq On : 28 Oct 2021 18:30
Operator : SY/MD
Sample : VV1028MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023082.D
Acq On : 28 Oct 2021 18:30
Operator : SY/MD
Sample : VV1028MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
