

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023083.D
 Acq On : 28 Oct 2021 18:54
 Operator : SY/MD
 Sample : VV1028MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

Signal : TIC: VV023083.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	143771	145069	13.30%	1.740%
2	1.568	157	164	176	rBV	115079	129660	11.89%	1.555%
3	2.108	322	332	349	rBV	241985	360719	33.08%	4.327%
4	2.365	407	412	414	rBV2	345	338	0.03%	0.004%
5	2.574	473	477	478	rBV	266	193	0.02%	0.002%
6	2.683	509	511	514	rBV3	287	225	0.02%	0.003%
7	2.760	532	535	537	rBV2	846	573	0.05%	0.007%
8	2.796	543	546	549	rBV2	284	206	0.02%	0.002%
9	3.121	645	647	652	rVB3	408	190	0.02%	0.002%
10	3.198	667	671	674	rBV2	502	313	0.03%	0.004%
11	3.217	674	677	681	rVB3	483	394	0.04%	0.005%
12	3.365	717	723	728	rBV	206	231	0.02%	0.003%
13	3.439	743	746	750	rVB	382	252	0.02%	0.003%
14	3.805	858	860	863	rBV	359	197	0.02%	0.002%
15	3.879	874	883	908	rBV	92858	248145	22.76%	2.976%
16	4.349	1014	1029	1051	rBV	178463	439239	40.28%	5.268%
17	4.619	1108	1113	1115	rBV3	562	467	0.04%	0.006%
18	4.632	1115	1117	1121	rBV3	479	229	0.02%	0.003%
19	4.715	1142	1143	1146	rBV2	408	210	0.02%	0.003%
20	4.735	1146	1149	1152	rBV2	370	235	0.02%	0.003%
21	4.921	1204	1207	1211	rBV3	292	244	0.02%	0.003%
22	5.047	1229	1246	1271	rBV2	422805	1090450	100.00%	13.079%
23	5.368	1342	1346	1349	rBV3	324	273	0.03%	0.003%
24	5.397	1353	1355	1357	rVB2	600	203	0.02%	0.002%
25	5.413	1357	1360	1361	rBV	550	250	0.02%	0.003%
26	5.497	1384	1386	1388	rVV	575	196	0.02%	0.002%
27	5.571	1403	1409	1411	rBV2	584	348	0.03%	0.004%
28	5.619	1412	1424	1446	rBV	317272	634065	58.15%	7.605%
29	5.918	1506	1517	1530	rVB7	3339	7763	0.71%	0.093%
30	6.072	1551	1565	1592	rBV	241628	499598	45.82%	5.992%
31	6.320	1639	1642	1646	rBV3	524	381	0.03%	0.005%
32	6.368	1653	1657	1660	rBV3	379	303	0.03%	0.004%
33	6.416	1670	1672	1677	rBV3	228	195	0.02%	0.002%
34	6.458	1681	1685	1689	rBV2	305	248	0.02%	0.003%
35	6.606	1727	1731	1734	rBV2	224	213	0.02%	0.003%
36	6.625	1734	1737	1740	rBV4	1252	1068	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023083.D
 Acq On : 28 Oct 2021 18:54
 Operator : SY/MD
 Sample : VV1028MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	6.850	1805	1807	1812	rVB3	327	320	0.03%	0.004%
38	6.944	1833	1836	1839	rBV3	340	229	0.02%	0.003%
39	6.989	1839	1850	1873	rBV	132174	242280	22.22%	2.906%
40	7.317	1939	1952	1971	rBV	496817	855550	78.46%	10.262%
41	7.567	2028	2030	2033	rVB3	720	375	0.03%	0.004%
42	7.622	2037	2047	2069	rBV	96242	167456	15.36%	2.009%
43	7.841	2113	2115	2117	rBV3	311	194	0.02%	0.002%
44	7.876	2124	2126	2130	rBV3	342	195	0.02%	0.002%
45	7.985	2155	2160	2165	rVV5	852	1033	0.09%	0.012%
46	8.088	2181	2192	2223	rBV	329950	558576	51.22%	6.700%
47	8.474	2306	2312	2317	rVB4	529	562	0.05%	0.007%
48	8.554	2335	2337	2340	rBV	526	226	0.02%	0.003%
49	8.609	2350	2354	2359	rVB3	538	521	0.05%	0.006%
50	8.632	2359	2361	2363	rBV3	388	224	0.02%	0.003%
51	8.853	2419	2430	2456	rBV	479502	777966	71.34%	9.331%
52	9.017	2478	2481	2485	rBV2	704	702	0.06%	0.008%
53	9.098	2502	2506	2507	rBV3	382	226	0.02%	0.003%
54	9.146	2515	2521	2524	rBV4	1014	1197	0.11%	0.014%
55	9.262	2551	2557	2564	rBV3	542	523	0.05%	0.006%
56	9.384	2592	2595	2598	rBV	362	238	0.02%	0.003%
57	9.403	2598	2601	2605	rVV2	256	208	0.02%	0.002%
58	9.426	2605	2608	2611	rVB2	670	357	0.03%	0.004%
59	9.519	2634	2637	2641	rBV2	307	201	0.02%	0.002%
60	9.548	2641	2646	2648	rBV3	576	410	0.04%	0.005%
61	9.828	2728	2733	2736	rBV3	314	257	0.02%	0.003%
62	9.847	2738	2739	2742	rVV	433	209	0.02%	0.003%
63	9.976	2776	2779	2782	rBV	292	206	0.02%	0.002%
64	10.127	2820	2826	2833	rVB5	2548	3549	0.33%	0.043%
65	10.217	2841	2854	2872	rBV	365697	566975	51.99%	6.801%
66	10.448	2922	2926	2928	rBV2	326	205	0.02%	0.002%
67	10.480	2933	2936	2939	rBV2	245	190	0.02%	0.002%
68	10.516	2944	2947	2951	rBV3	399	251	0.02%	0.003%
69	10.541	2951	2955	2958	rBV2	802	549	0.05%	0.007%
70	10.664	2989	2993	2994	rBV3	385	211	0.02%	0.003%
71	10.834	3044	3046	3051	rBV2	293	212	0.02%	0.003%
72	10.921	3060	3073	3083	rBV4	3232	5017	0.46%	0.060%
73	10.969	3086	3088	3091	rBV	283	204	0.02%	0.002%
74	11.024	3101	3105	3108	rBV	632	504	0.05%	0.006%
75	11.185	3151	3155	3165	rBV6	1326	2020	0.19%	0.024%
76	11.249	3165	3175	3192	rBV	489067	753979	69.14%	9.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023083.D
 Acq On : 28 Oct 2021 18:54
 Operator : SY/MD
 Sample : VV1028MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

77	11.461	3238	3241	3244	rVB2	496	286	0.03%	0.003%
78	11.564	3268	3273	3275	rBV2	405	298	0.03%	0.004%
79	11.625	3280	3292	3310	rBV	519663	808948	74.18%	9.703%
80	11.786	3339	3342	3348	rVB4	1175	1225	0.11%	0.015%
81	11.873	3367	3369	3371	rVB2	636	196	0.02%	0.002%
82	11.969	3395	3399	3401	rBV	463	419	0.04%	0.005%
83	12.001	3407	3409	3414	rVB2	453	282	0.03%	0.003%
84	12.094	3436	3438	3439	rBV2	496	228	0.02%	0.003%
85	12.541	3574	3577	3582	rBV3	411	364	0.03%	0.004%
86	12.651	3604	3611	3619	rBV5	2440	3452	0.32%	0.041%
87	12.850	3671	3673	3678	rVB4	728	402	0.04%	0.005%
88	12.937	3698	3700	3706	rVB3	466	444	0.04%	0.005%
89	13.197	3777	3781	3784	rVB3	431	282	0.03%	0.003%
90	13.271	3796	3804	3811	rBV6	2931	3861	0.35%	0.046%
91	13.313	3814	3817	3820	rBV2	488	311	0.03%	0.004%
92	13.509	3871	3878	3889	rBV2	2591	3992	0.37%	0.048%
93	13.660	3920	3925	3926	rBV2	309	271	0.02%	0.003%
94	13.699	3934	3937	3941	rBV3	467	345	0.03%	0.004%
95	13.750	3948	3953	3960	rVB5	2165	2603	0.24%	0.031%
96	13.934	4007	4010	4014	rBV4	507	466	0.04%	0.006%
97	14.223	4098	4100	4103	rVB2	398	210	0.02%	0.003%
98	14.467	4174	4176	4180	rBV2	573	488	0.04%	0.006%
99	15.085	4366	4368	4371	rVV3	637	372	0.03%	0.004%
100	15.184	4396	4399	4401	rBV2	558	260	0.02%	0.003%




Sum of corrected areas: 8337195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023083.D
Acq On : 28 Oct 2021 18:54
Operator : SY/MD
Sample : VV1028MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

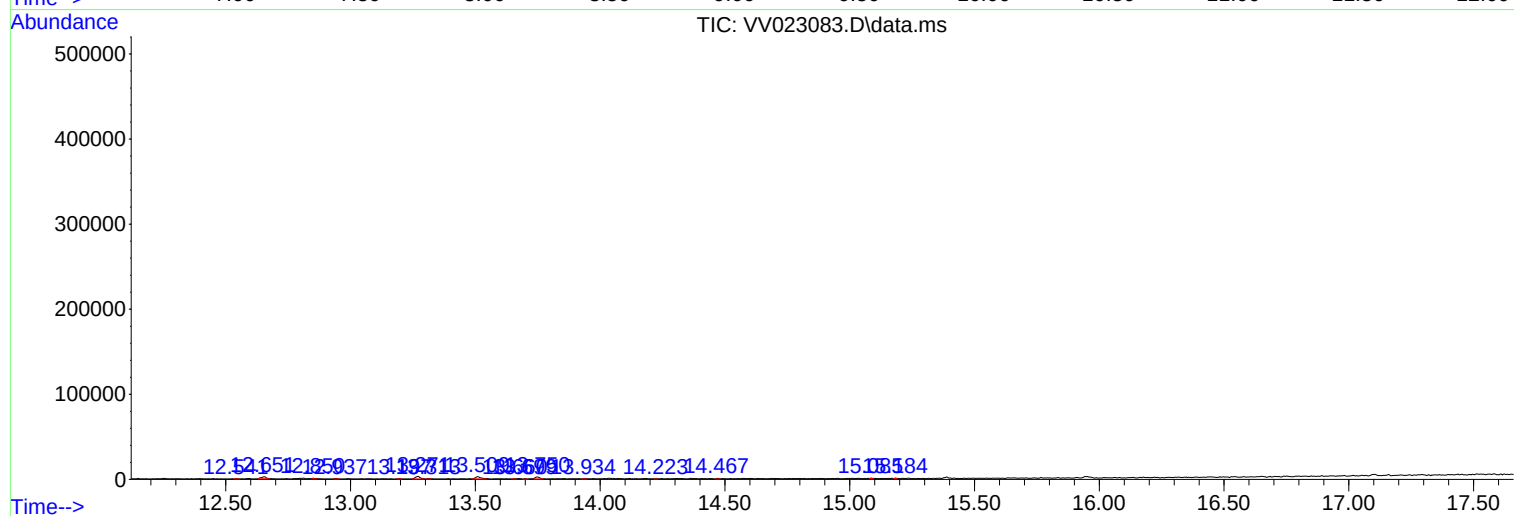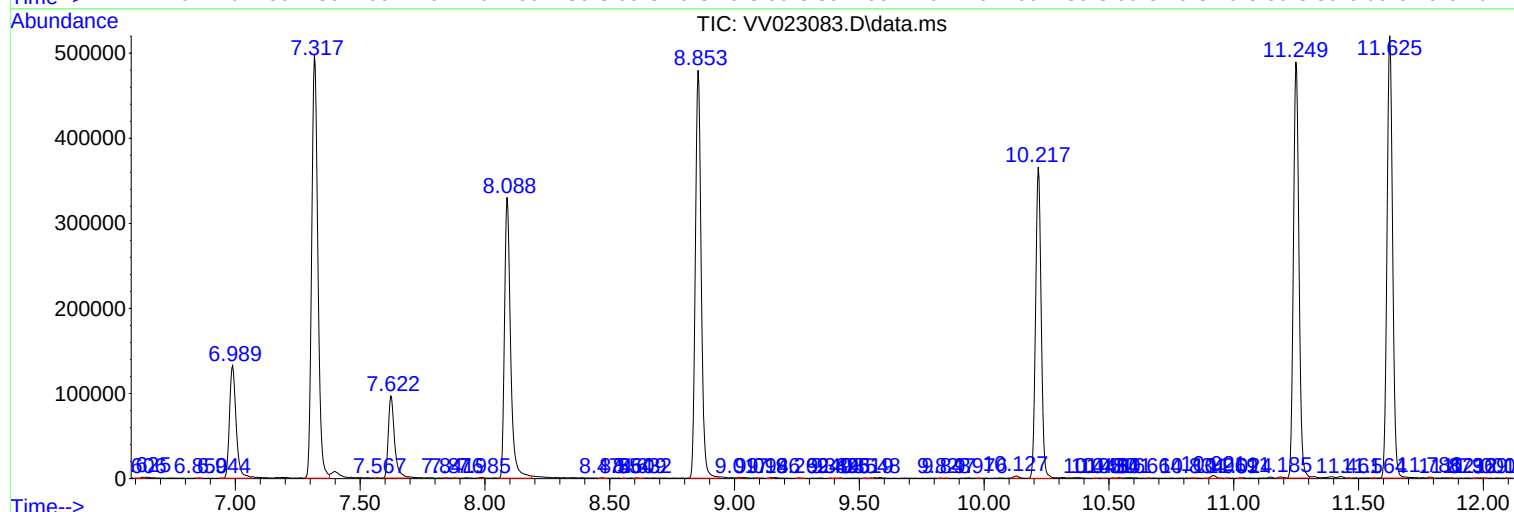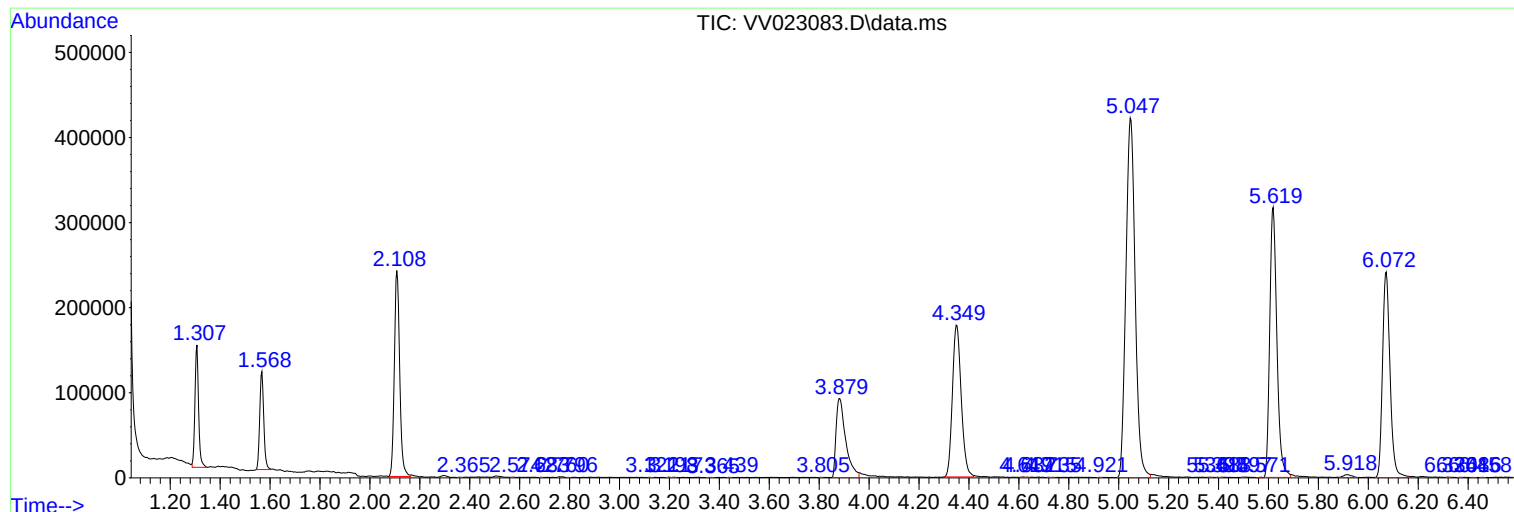

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023083.D
Acq On : 28 Oct 2021 18:54
Operator : SY/MD
Sample : VV1028MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023083.D
Acq On : 28 Oct 2021 18:54
Operator : SY/MD
Sample : VV1028MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
