

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023084.D
 Acq On : 28 Oct 2021 19:18
 Operator : SY/MD
 Sample : VV1028WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

Signal : TIC: VV023084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	97	rVB	138673	145610	13.53%	1.764%
2	1.564	157	163	179	rVB	114489	133044	12.36%	1.612%
3	2.108	322	332	356	rVB	241939	356325	33.11%	4.317%
4	2.384	415	418	420	rBV3	593	431	0.04%	0.005%
5	2.436	432	434	436	rVV	405	209	0.02%	0.003%
6	2.603	483	486	491	rBV2	393	317	0.03%	0.004%
7	3.053	623	626	629	rBV	345	219	0.02%	0.003%
8	3.172	659	663	665	rBV2	232	201	0.02%	0.002%
9	3.481	756	759	763	rBV3	318	287	0.03%	0.003%
10	3.503	763	766	767	rVV2	339	194	0.02%	0.002%
11	3.712	828	831	834	rBV2	318	208	0.02%	0.003%
12	3.879	873	883	914	rBV	92226	245190	22.78%	2.970%
13	4.349	1013	1029	1058	rBV	177340	437514	40.66%	5.300%
14	4.693	1133	1136	1140	rVB3	659	448	0.04%	0.005%
15	4.780	1159	1163	1166	rBV3	241	213	0.02%	0.003%
16	4.883	1191	1195	1197	rBV	308	231	0.02%	0.003%
17	5.047	1229	1246	1271	rBV2	417951	1076153	100.00%	13.038%
18	5.429	1363	1365	1367	rBV2	465	254	0.02%	0.003%
19	5.522	1392	1394	1397	rBV2	383	235	0.02%	0.003%
20	5.619	1408	1424	1449	rBV	313980	638459	59.33%	7.735%
21	5.799	1478	1480	1484	rBV3	428	207	0.02%	0.003%
22	5.915	1504	1516	1530	rVB9	3496	8525	0.79%	0.103%
23	6.072	1549	1565	1591	rBV	243163	493591	45.87%	5.980%
24	6.252	1619	1621	1627	rVB3	945	635	0.06%	0.008%
25	6.513	1699	1702	1705	rBV2	330	191	0.02%	0.002%
26	6.535	1705	1709	1710	rBV	463	260	0.02%	0.003%
27	6.741	1768	1773	1775	rBV2	307	207	0.02%	0.003%
28	6.796	1785	1790	1793	rBV2	407	200	0.02%	0.002%
29	6.883	1814	1817	1820	rVB2	310	208	0.02%	0.003%
30	6.985	1837	1849	1870	rBV	129746	238707	22.18%	2.892%
31	7.268	1933	1937	1940	rBV2	381	201	0.02%	0.002%
32	7.317	1940	1952	1970	rBV	487156	848732	78.87%	10.282%
33	7.583	2033	2035	2038	rBV	345	207	0.02%	0.003%
34	7.622	2038	2047	2074	rVV	93293	164591	15.29%	1.994%
35	7.850	2116	2118	2121	rVB2	467	227	0.02%	0.003%
36	7.873	2121	2125	2128	rVB2	377	220	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023084.D
 Acq On : 28 Oct 2021 19:18
 Operator : SY/MD
 Sample : VV1028WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis

37	7.931	2141	2143	2151	rBV3	424	485	0.05%	0.006%
38	8.046	2172	2179	2180	rBV2	386	372	0.03%	0.005%
39	8.088	2180	2192	2215	rBV	324299	541745	50.34%	6.563%
40	8.403	2288	2290	2294	rVB2	305	204	0.02%	0.002%
41	8.448	2301	2304	2310	rVB2	419	352	0.03%	0.004%
42	8.497	2316	2319	2321	rBV	385	284	0.03%	0.003%
43	8.532	2328	2330	2333	rBV3	456	262	0.02%	0.003%
44	8.567	2340	2341	2346	rVB2	676	369	0.03%	0.004%
45	8.596	2347	2350	2355	rBV3	536	547	0.05%	0.007%
46	8.780	2405	2407	2411	rVB3	367	272	0.03%	0.003%
47	8.854	2418	2430	2457	rBV	488393	786461	73.08%	9.528%
48	9.143	2514	2520	2522	rBV3	1117	905	0.08%	0.011%
49	9.394	2595	2598	2601	rVV3	301	248	0.02%	0.003%
50	9.413	2601	2604	2609	rVV3	343	324	0.03%	0.004%
51	9.500	2625	2631	2633	rBV2	244	248	0.02%	0.003%
52	9.545	2643	2645	2649	rBV	610	431	0.04%	0.005%
53	9.577	2652	2655	2660	rVV2	483	365	0.03%	0.004%
54	9.741	2702	2706	2710	rBV3	322	263	0.02%	0.003%
55	9.776	2714	2717	2719	rVB2	446	213	0.02%	0.003%
56	9.841	2733	2737	2739	rBV2	388	225	0.02%	0.003%
57	9.902	2754	2756	2760	rVV3	482	238	0.02%	0.003%
58	9.934	2764	2766	2773	rVV3	499	476	0.04%	0.006%
59	9.960	2773	2774	2778	rVB3	473	232	0.02%	0.003%
60	10.127	2818	2826	2837	rVB2	2205	3750	0.35%	0.045%
61	10.217	2841	2854	2874	rBV	360107	555158	51.59%	6.726%
62	10.313	2882	2884	2887	rBV5	657	461	0.04%	0.006%
63	10.503	2939	2943	2946	rBV3	388	280	0.03%	0.003%
64	10.538	2950	2954	2955	rBV3	581	350	0.03%	0.004%
65	10.603	2972	2974	2982	rVB3	739	780	0.07%	0.009%
66	10.644	2982	2987	2990	rBV2	244	290	0.03%	0.004%
67	10.670	2992	2995	2997	rBV3	596	290	0.03%	0.004%
68	10.831	3042	3045	3048	rBV2	382	258	0.02%	0.003%
69	10.915	3064	3071	3080	rBV5	2570	3513	0.33%	0.043%
70	11.030	3101	3107	3108	rBV2	367	320	0.03%	0.004%
71	11.062	3113	3117	3119	rBV2	399	322	0.03%	0.004%
72	11.149	3137	3144	3147	rBV5	1241	1443	0.13%	0.017%
73	11.249	3164	3175	3195	rBV	494276	751302	69.81%	9.102%
74	11.567	3271	3274	3275	rBV	654	313	0.03%	0.004%
75	11.625	3280	3292	3314	rBV	506772	791055	73.51%	9.584%
76	11.934	3383	3388	3389	rBV	614	457	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023084.D
 Acq On : 28 Oct 2021 19:18
 Operator : SY/MD
 Sample : VV1028WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M

Title : VOC Analysis

77	11.969	3396	3399	3401	rVB2	449	237	0.02%	0.003%
78	11.985	3401	3404	3407	rBV2	390	304	0.03%	0.004%
79	12.040	3419	3421	3425	rBV2	443	305	0.03%	0.004%
80	12.095	3433	3438	3443	rBV3	626	616	0.06%	0.007%
81	12.239	3480	3483	3485	rBV2	496	340	0.03%	0.004%
82	12.374	3522	3525	3528	rVB	404	217	0.02%	0.003%
83	12.503	3562	3565	3567	rVB2	390	203	0.02%	0.002%
84	12.599	3590	3595	3599	rVB2	490	462	0.04%	0.006%
85	12.651	3607	3611	3613	rBV3	1461	1365	0.13%	0.017%
86	12.747	3637	3641	3645	rBV2	620	485	0.05%	0.006%
87	12.847	3669	3672	3679	rVB4	661	499	0.05%	0.006%
88	12.885	3680	3684	3686	rBV	383	217	0.02%	0.003%
89	13.123	3756	3758	3762	rVB3	474	203	0.02%	0.002%
90	13.271	3797	3804	3811	rVB5	1898	2453	0.23%	0.030%
91	13.348	3824	3828	3832	rBV3	316	329	0.03%	0.004%
92	13.397	3841	3843	3850	rVB3	471	356	0.03%	0.004%
93	13.554	3890	3892	3897	rVB2	508	304	0.03%	0.004%
94	13.750	3945	3953	3960	rBV2	1686	2246	0.21%	0.027%
95	13.808	3968	3971	3972	rBV3	411	240	0.02%	0.003%
96	14.030	4037	4040	4041	rBV3	578	315	0.03%	0.004%
97	14.345	4135	4138	4140	rBV2	465	231	0.02%	0.003%
98	14.583	4210	4212	4216	rBV2	418	262	0.02%	0.003%
99	15.860	4607	4609	4611	rBV	706	277	0.03%	0.003%
100	15.950	4632	4637	4643	rBV6	2730	3300	0.31%	0.040%




Sum of corrected areas: 8254280

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023084.D
Acq On : 28 Oct 2021 19:18
Operator : SY/MD
Sample : VV1028WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

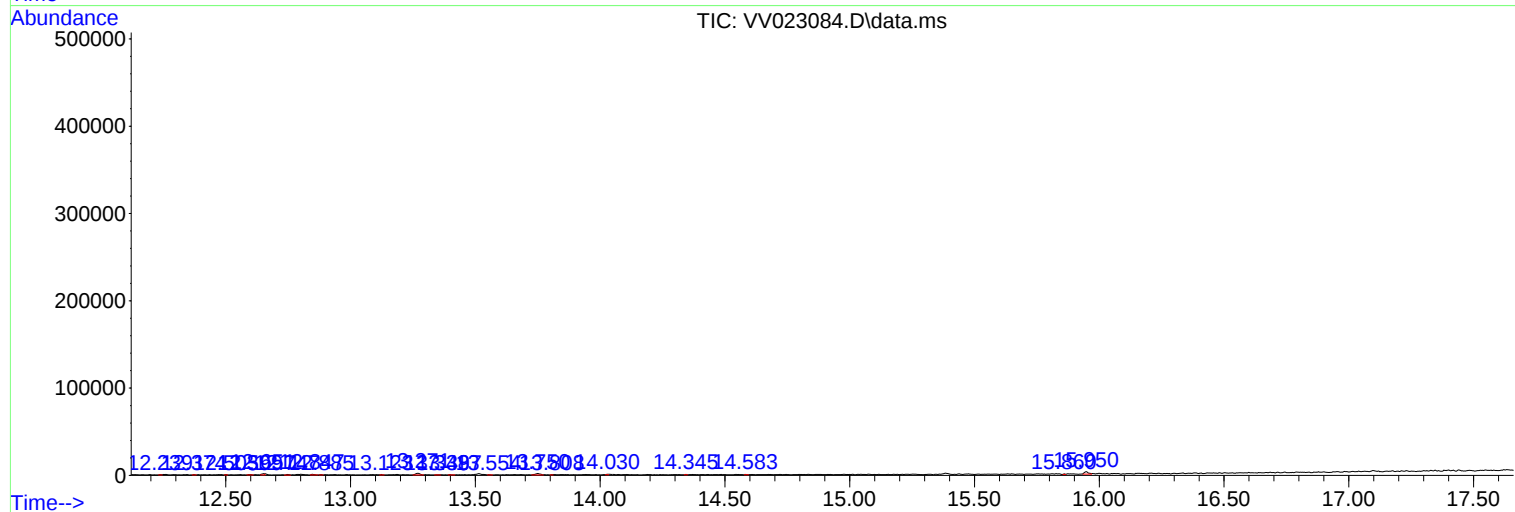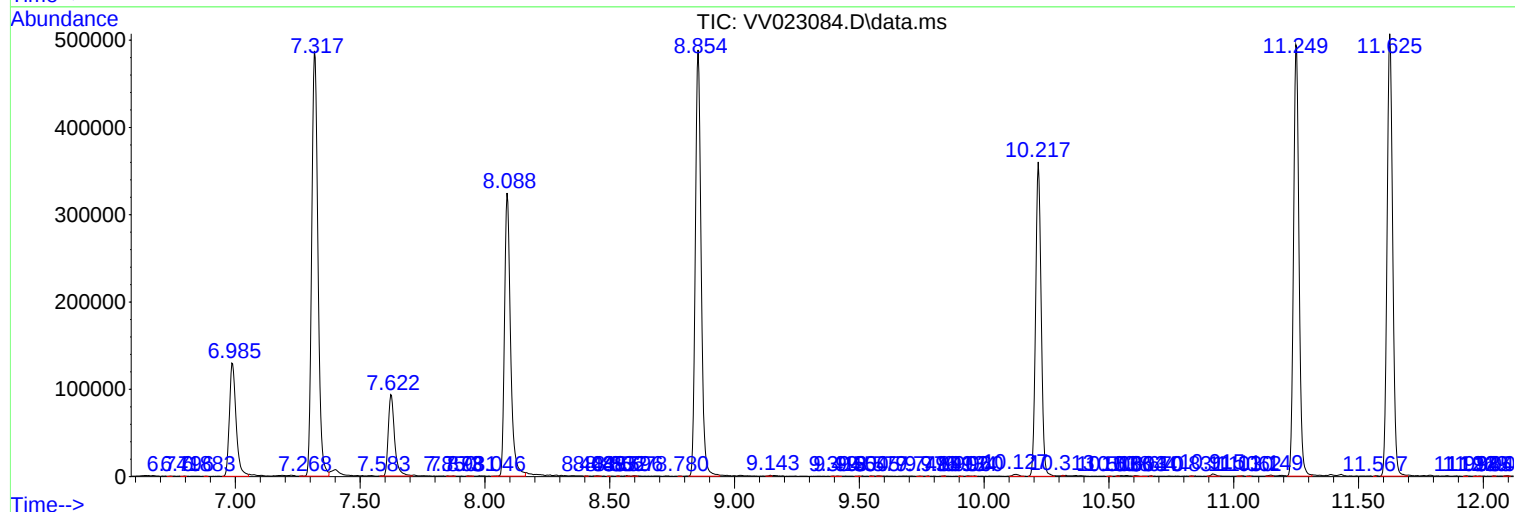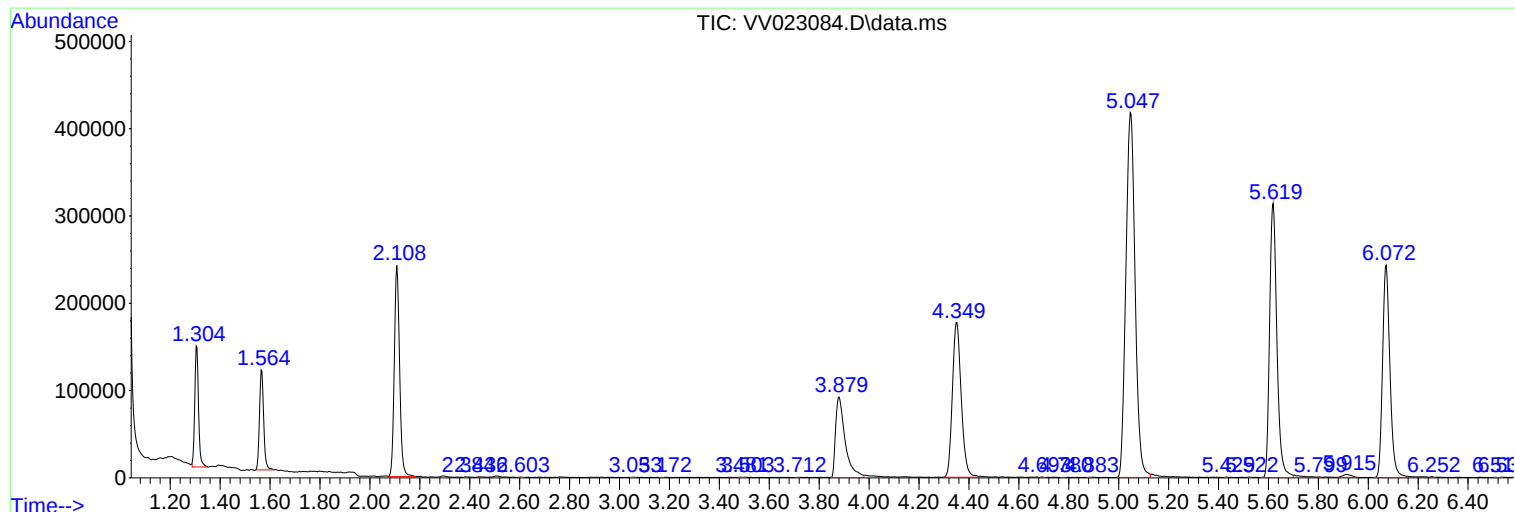

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023084.D
Acq On : 28 Oct 2021 19:18
Operator : SY/MD
Sample : VV1028WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
Data File : VV023084.D
Acq On : 28 Oct 2021 19:18
Operator : SY/MD
Sample : VV1028WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK266

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
