
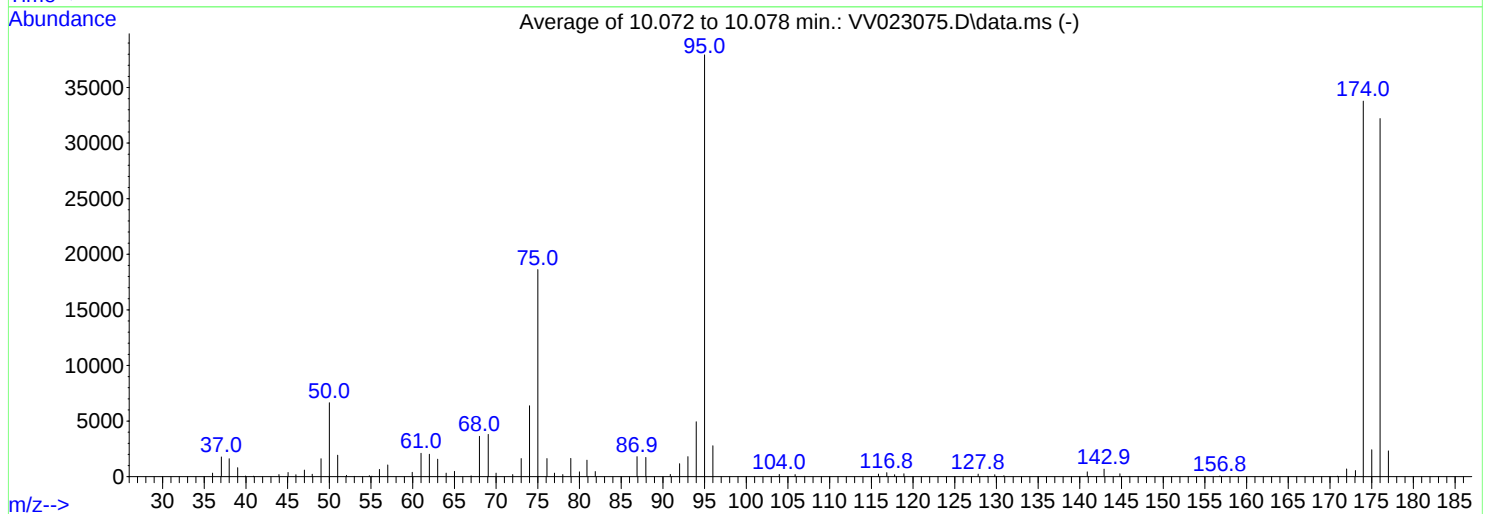


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102821\
 Data File : VV023075.D
 Acq On : 28 Oct 2021 14:57
 Operator : SY/MD
 Sample : BFB243
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB243

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM102821WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 30 00:25:16 2021

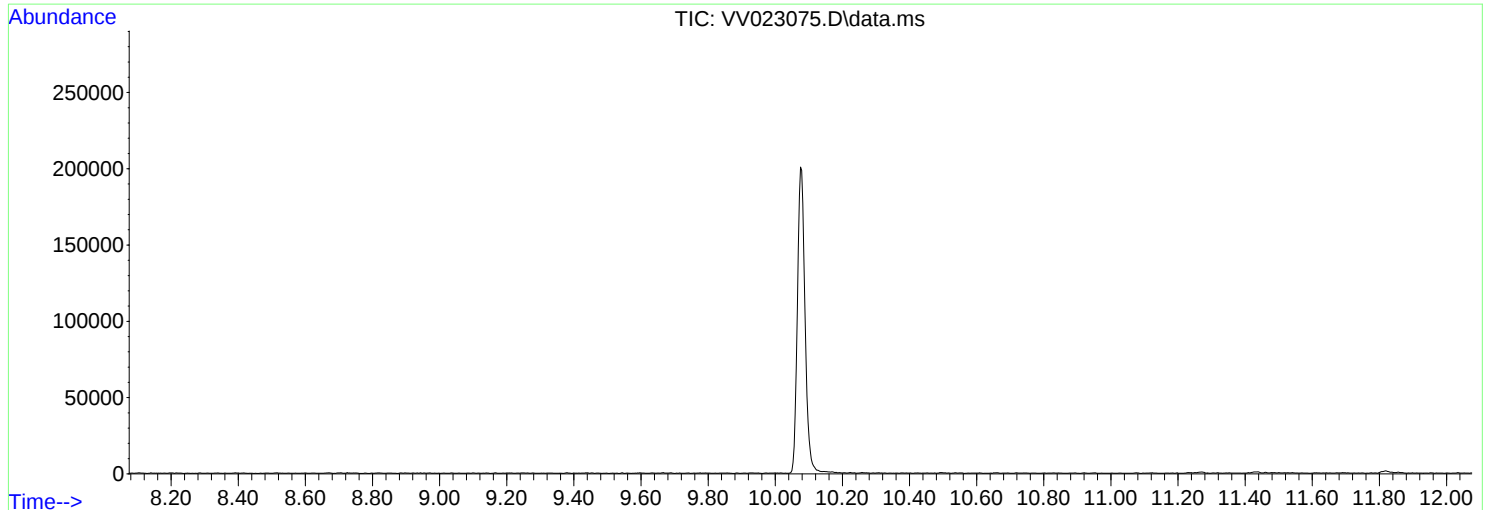

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6653	PASS
75	95	30	80	49.1	18624	PASS
95	95	100	100	100.0	37939	PASS
96	95	5	9	7.3	2775	PASS
173	174	0.00	2	1.6	544	PASS
174	95	50	120	89.0	33784	PASS
175	174	5	9	7.2	2424	PASS
176	174	95	105	95.3	32203	PASS
177	176	5	10	7.2	2312	PASS

m/z	Abundance
36.00	344.0
37.00	1880.0
38.00	1596.0
39.00	844.0
40.00	240.0
44.00	475.0
45.00	368.0
46.00	181.0
47.00	593.0
47.90	209.0
49.00	1540.0
50.00	6683.0
51.00	1918.0
52.10	118.0
53.00	105.0
55.10	133.0
56.00	675.0
57.00	1075.0
59.90	424.0
61.00	2220.0
62.00	2086.0
63.00	1555.0
64.00	293.0
65.00	502.0
67.00	108.0
68.00	3745.0
69.10	3811.0
70.00	301.0
72.00	194.0
73.00	1610.0
74.00	6270.0
75.00	18616.0
76.10	1659.0
77.00	314.0
78.00	203.0
78.90	1680.0
80.00	423.0
80.90	1513.0
81.90	464.0
86.90	1807.0
88.00	1878.0
90.90	206.0
92.00	1251.0
93.00	1883.0
94.00	4981.0
95.00	38424.0
96.00	2723.0
104.00	208.0
105.80	191.0
107.00	103.0
115.80	214.0
116.90	374.0
117.80	163.0
118.90	281.0
127.70	231.0
128.90	106.0
129.80	161.0
130.90	142.0
140.90	444.0
142.90	670.0
144.80	254.0
145.90	106.0
154.90	107.0
170.90	114.0
172.00	795.0
173.10	550.0
174.00	35320.0
175.00	2460.0
176.00	33600.0
177.00	2230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
39.90	192.0
43.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.00	299.0
37.10	1591.0
38.00	1601.0
39.00	736.0
40.00	260.0
40.90	138.0
44.00	432.0
45.10	347.0
46.00	148.0
47.00	556.0
48.00	222.0
49.00	1640.0
50.00	6429.0
51.00	1876.0
52.00	101.0
54.80	139.0
56.00	585.0
57.00	990.0
60.00	333.0
61.00	1895.0
62.00	1858.0
63.00	1495.0
64.00	326.0
65.00	433.0
68.00	3355.0
69.00	3659.0
70.00	341.0
72.00	198.0
73.00	1546.0
74.00	6251.0
75.00	17872.0
76.10	1566.0
77.00	291.0
78.00	174.0
79.00	1576.0
80.00	420.0
80.90	1395.0
81.90	429.0
86.90	1734.0
87.90	1531.0
90.90	180.0
92.00	1054.0
93.00	1677.0
94.00	4648.0
95.00	35984.0
96.00	2709.0
103.90	204.0
105.90	178.0
115.90	213.0
116.80	325.0
117.80	167.0
118.90	247.0
127.90	223.0
129.80	174.0
140.90	410.0
142.90	653.0
144.80	232.0
156.80	119.0
172.00	563.0
173.00	507.0
174.00	31200.0
175.00	2311.0
176.00	29584.0
177.00	2289.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.00	319.0
37.00	1828.0
38.00	1646.0
39.00	836.0
40.00	266.0
44.00	455.0
45.10	401.0
46.00	215.0
47.00	609.0
47.90	224.0
49.00	1664.0
50.00	6846.0
51.00	2016.0
52.00	110.0
54.80	132.0
56.00	684.0
57.00	1099.0
60.00	392.0
61.00	2174.0
62.00	2100.0
63.00	1645.0
64.00	323.0
65.00	509.0
67.00	106.0
68.00	3784.0
69.00	3919.0
70.00	316.0
72.00	172.0
73.00	1722.0
74.00	6595.0
75.00	19384.0
76.10	1671.0
77.00	330.0
78.00	169.0
79.00	1691.0
80.00	440.0
80.90	1544.0
81.90	496.0
86.90	1869.0
87.90	1789.0
90.90	205.0
92.00	1194.0
93.00	1841.0
94.00	5172.0
95.00	39408.0
96.00	2893.0
104.00	210.0
105.90	182.0
115.90	254.0
116.80	363.0
117.80	168.0
118.90	263.0
127.80	224.0
129.80	169.0
130.90	105.0
140.90	437.0
142.90	717.0
144.80	286.0
156.80	108.0
172.00	720.0
173.00	574.0
174.00	34832.0
175.00	2502.0
176.00	33424.0
177.00	2417.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243