

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102822\
 Data File : VW028752.D
 Acq On : 28 Oct 2022 13:20
 Operator : SY/MD
 Sample : N5232-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAC6

Quant Time: Oct 28 21:52:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 28 21:50:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	182548	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	168743	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	74755	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44519	3.507	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.200%
7) Chloroethane-d5	1.565	69	44822	4.175	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.600%
11) 1,1-Dichloroethene-d2	2.105	63	72176	2.939	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.800%#
20) 2-Butanone-d5	3.908	46	163409	56.446	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.900%
24) Chloroform-d	4.346	84	94875	4.304	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.034	65	52994	4.737	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
32) Benzene-d6	5.047	84	181941	4.032	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.600%
36) 1,2-Dichloropropane-d6	6.069	67	67664	4.737	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.313	98	143936	4.088	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	7.622	79	14929	3.364	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.200%
46) 2-Hexanone-d5	8.092	63	114287	55.321	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.640%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	47456	5.009	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.200%
66) 1,2-Dichlorobenzene-d4	11.619	152	49681	4.818	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						Qvalue
25) Chloroform	4.378	83	7000	0.295	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028752.D
Acq On : 28 Oct 2022 13:20
Operator : SY/MD
Sample : N5232-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAC6

Quant Time: Oct 28 21:52:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 28 21:50:06 2022
Response via : Initial Calibration

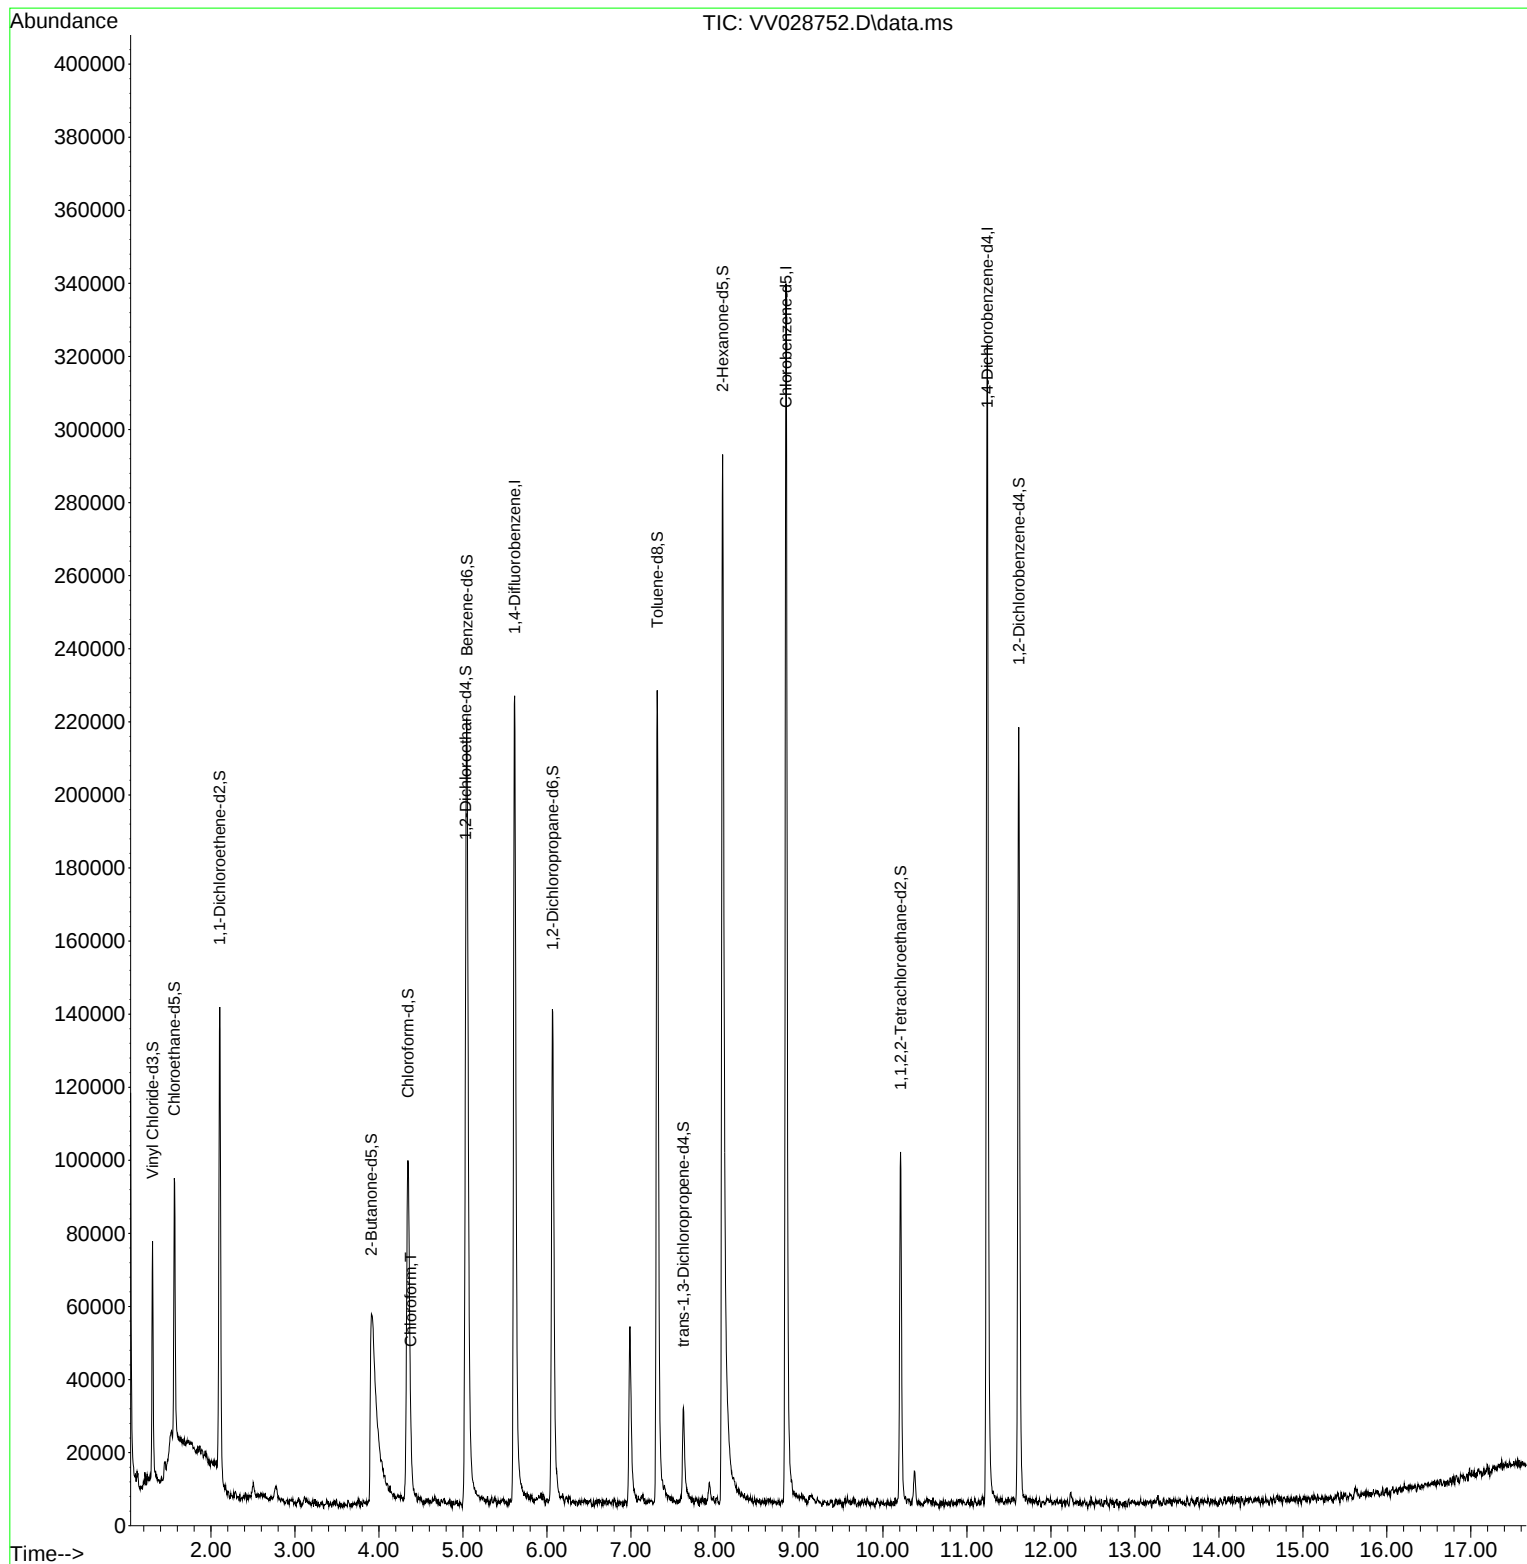

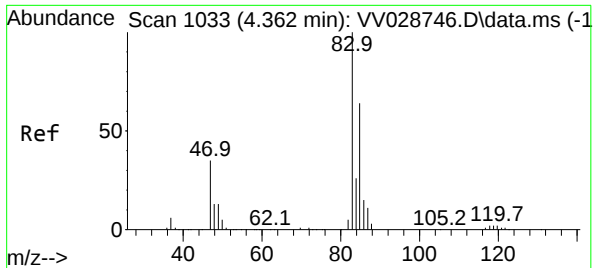

#25
 Chloroform
 Concen: 0.295 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.016 min
 Lab File: VV028752.D
 Acq: 28 Oct 2022 13:20

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAC6

Tgt Ion: 83 Resp: 7000
 Ion Ratio Lower Upper
 83 100
 85 73.7 44.1 81.9

