

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028753.D
 Acq On : 28 Oct 2022 13:44
 Operator : SY/MD
 Sample : N5232-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rBV	100662	108253	17.57%	2.053%
2	1.449	120	127	131	rBV8	6976	7894	1.28%	0.150%
3	1.564	156	163	173	rBV	90017	106762	17.33%	2.025%
4	2.105	321	331	347	rVB	184613	260984	42.37%	4.950%
5	3.905	876	891	914	rBV	38267	144485	23.46%	2.740%
6	4.349	1013	1029	1055	rBV4	124909	425293	69.05%	8.067%
7	5.043	1227	1245	1267	rBV3	241062	615952	100.00%	11.683%
8	5.612	1411	1422	1442	rBV	223775	457506	74.28%	8.678%
9	6.066	1550	1563	1586	rBV2	138207	297418	48.29%	5.641%
10	6.985	1837	1849	1866	rBV2	51107	105425	17.12%	2.000%
11	7.313	1937	1951	1970	rBV	268119	498698	80.96%	9.459%
12	7.394	1970	1976	1986	rVB	15271	26857	4.36%	0.509%
13	7.622	2038	2047	2063	rBV2	25886	52213	8.48%	0.990%
14	7.940	2137	2146	2152	rVB5	6379	10351	1.68%	0.196%
15	8.091	2180	2193	2224	rBV	207143	517425	84.00%	9.814%
16	8.847	2414	2428	2452	rBV	331796	572079	92.88%	10.851%
17	9.143	2508	2520	2524	rBV7	8719	15110	2.45%	0.287%
18	10.210	2840	2852	2868	rBV	84324	136447	22.15%	2.588%
19	10.378	2894	2904	2913	rBV3	11441	19575	3.18%	0.371%
20	11.242	3161	3173	3192	rBV	315955	517130	83.96%	9.808%
21	11.615	3276	3289	3306	rBV	219564	365606	59.36%	6.934%
22	12.345	3508	3516	3524	rBV	6524	10855	1.76%	0.206%




Sum of corrected areas: 5272318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028753.D
Acq On : 28 Oct 2022 13:44
Operator : SY/MD
Sample : N5232-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

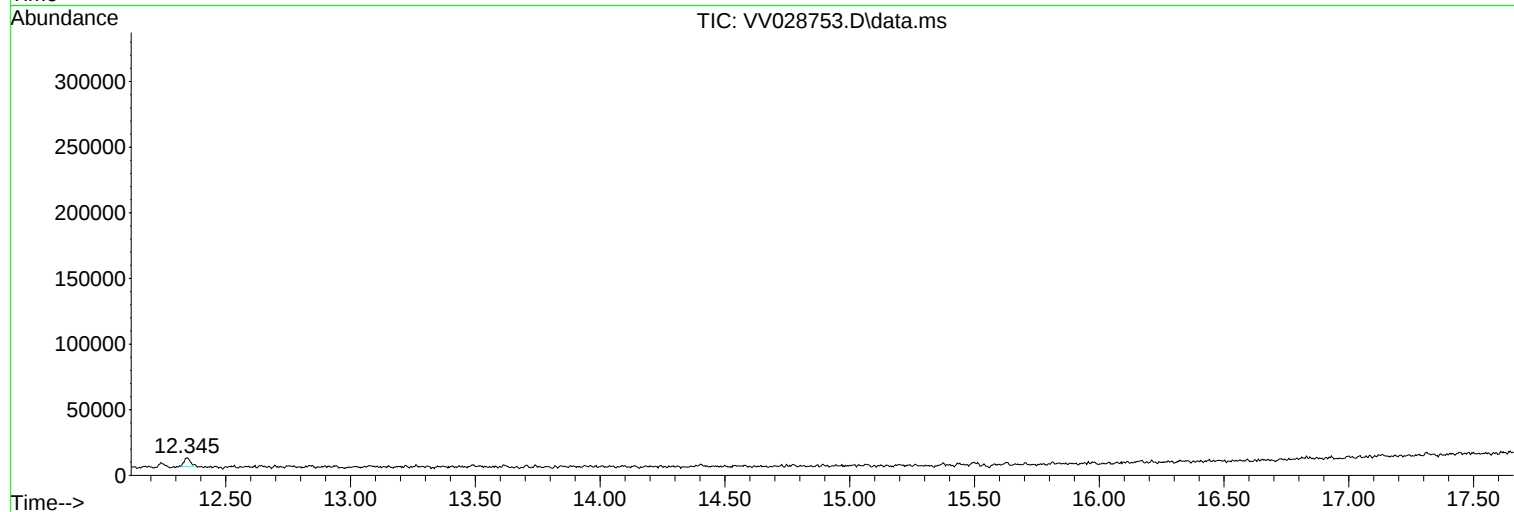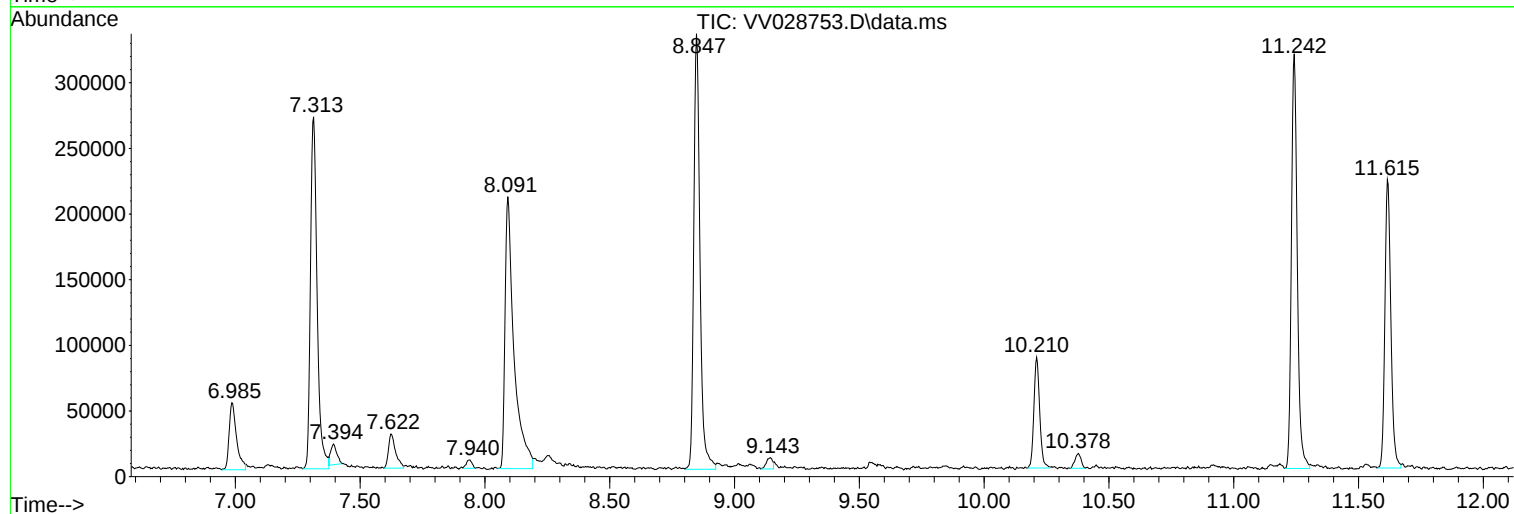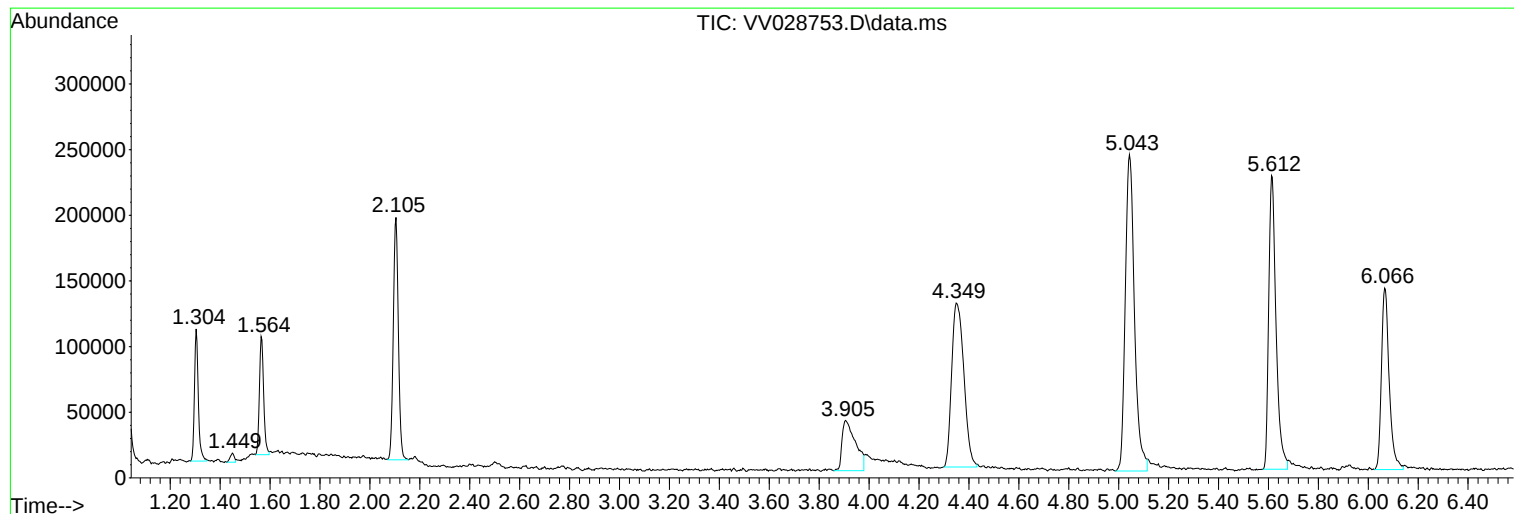

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028753.D
Acq On : 28 Oct 2022 13:44
Operator : SY/MD
Sample : N5232-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028753.D
Acq On : 28 Oct 2022 13:44
Operator : SY/MD
Sample : N5232-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc