

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028754.D
 Acq On : 28 Oct 2022 14:06
 Operator : SY/MD
 Sample : N5232-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAD4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rBV	99519	106118	18.04%	2.083%
2	1.568	157	164	175	rVB	87816	100216	17.04%	1.967%
3	2.105	322	331	347	rVB	180213	261929	44.54%	5.141%
4	3.918	883	895	923	rBV2	32501	139066	23.65%	2.730%
5	4.355	1012	1031	1054	rBV4	118451	409838	69.69%	8.044%
6	5.047	1228	1246	1275	rBV3	228896	588082	100.00%	11.543%
7	5.616	1410	1423	1450	rBV	218436	462365	78.62%	9.075%
8	6.069	1547	1564	1587	rBV2	136488	294240	50.03%	5.775%
9	6.989	1837	1850	1866	rBV2	49914	99146	16.86%	1.946%
10	7.313	1938	1951	1968	rBV	256658	463660	78.84%	9.101%
11	7.394	1969	1976	1990	rVB2	13314	30511	5.19%	0.599%
12	7.625	2037	2048	2060	rBV3	25107	47252	8.03%	0.927%
13	7.934	2133	2144	2154	rBV4	7987	15557	2.65%	0.305%
14	8.092	2182	2193	2231	rBV	186680	499694	84.97%	9.808%
15	8.847	2413	2428	2452	rBV	329262	563636	95.84%	11.063%
16	9.140	2511	2519	2520	rBV8	7222	7330	1.25%	0.144%
17	10.210	2841	2852	2873	rVB	78956	135134	22.98%	2.652%
18	10.378	2895	2904	2914	rVB4	12430	19896	3.38%	0.391%
19	11.243	3162	3173	3191	rBV	311237	499242	84.89%	9.799%
20	11.619	3278	3290	3303	rBV	210617	344548	58.59%	6.763%
21	12.349	3510	3517	3521	rBV8	5919	7203	1.22%	0.141%




Sum of corrected areas: 5094663

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028754.D
Acq On : 28 Oct 2022 14:06
Operator : SY/MD
Sample : N5232-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

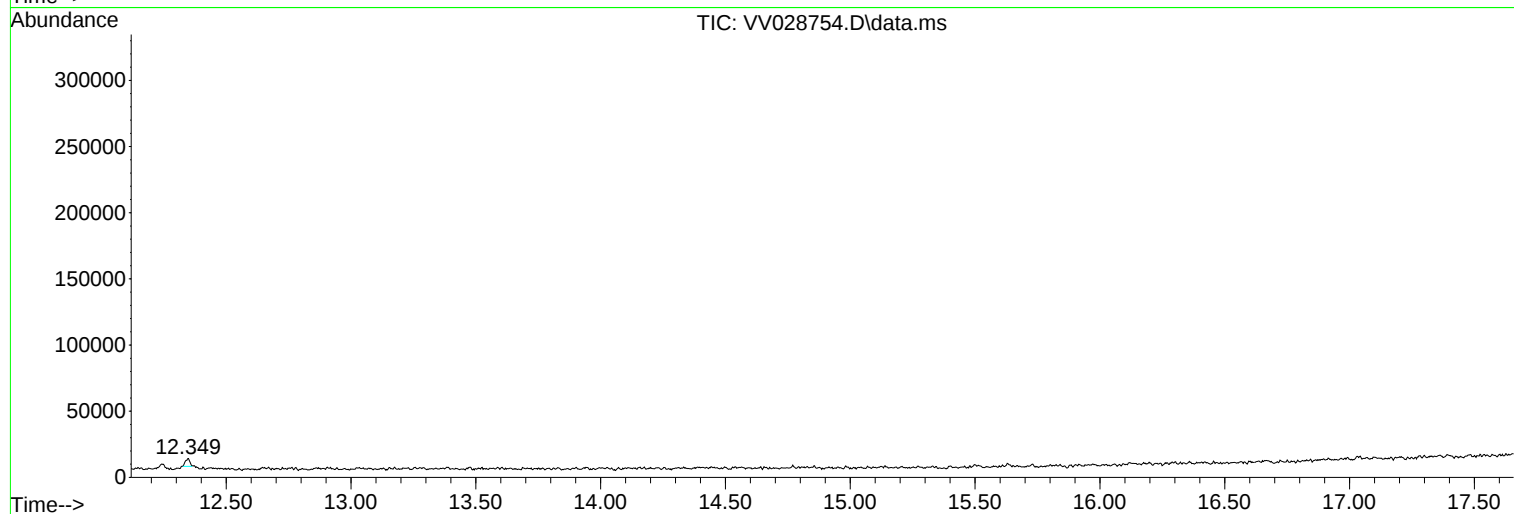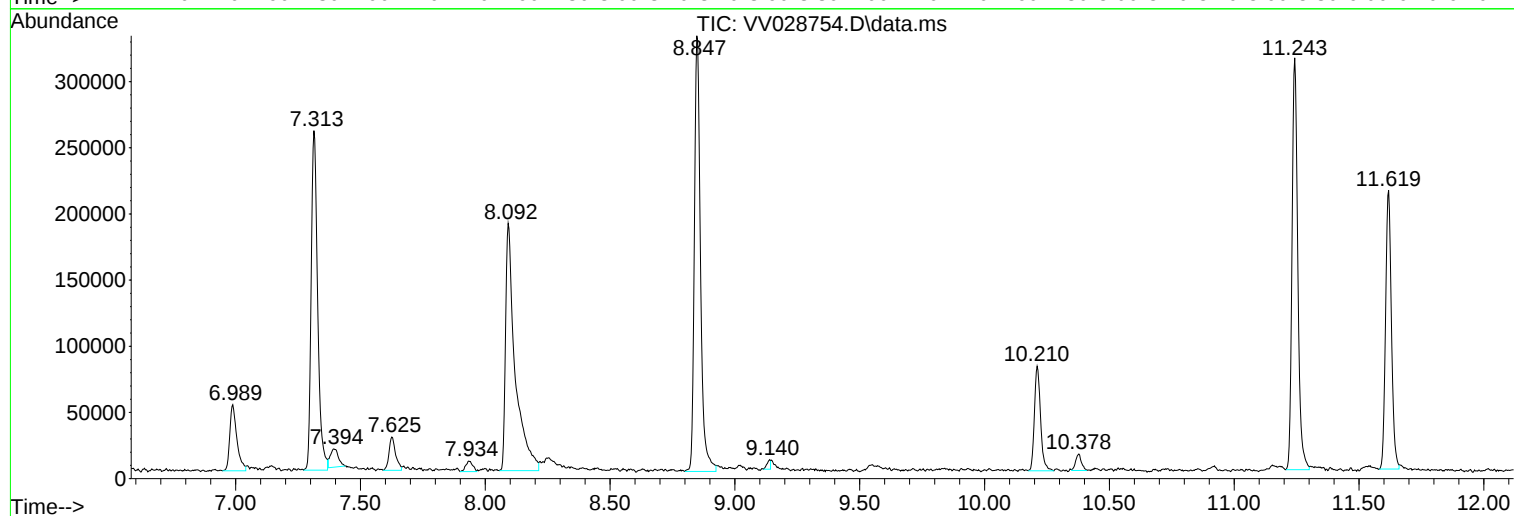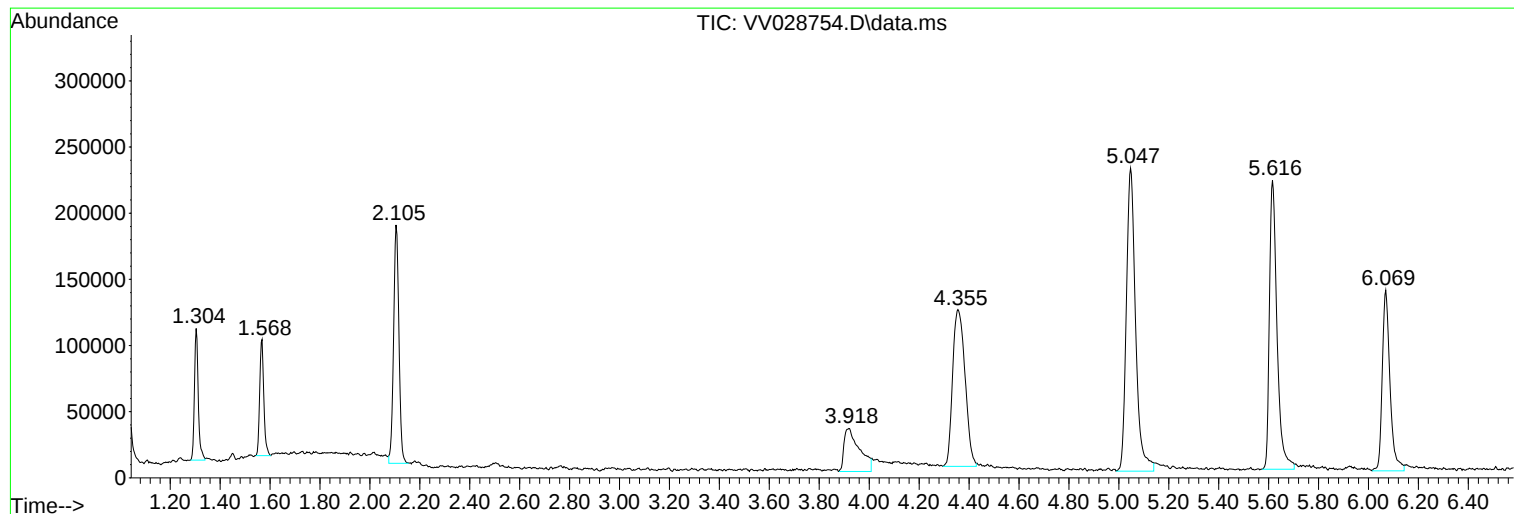

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028754.D
Acq On : 28 Oct 2022 14:06
Operator : SY/MD
Sample : N5232-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028754.D
Acq On : 28 Oct 2022 14:06
Operator : SY/MD
Sample : N5232-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
