

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028755.D
 Acq On : 28 Oct 2022 14:31
 Operator : SY/MD
 Sample : N5233-08DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA76DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.131	25	28	35	rVB	8011	8200	1.20%	0.136%
2	1.304	74	82	97	rBV2	71634	82558	12.07%	1.365%
3	1.568	157	164	173	rBV	72260	79586	11.64%	1.315%
4	2.105	322	331	353	rVB	131179	202967	29.68%	3.355%
5	2.503	445	455	467	rBV	17880	31027	4.54%	0.513%
6	3.757	841	845	856	rVB10	5274	8961	1.31%	0.148%
7	3.905	875	891	921	rBV3	126314	433492	63.39%	7.165%
8	4.346	1013	1028	1049	rBV	92651	233387	34.13%	3.858%
9	5.044	1228	1245	1253	rBV2	221106	523130	76.50%	8.647%
10	5.095	1253	1261	1289	rVB2	295317	683853	100.00%	11.303%
11	5.613	1412	1422	1449	rBV2	218583	453432	66.31%	7.495%
12	6.066	1549	1563	1591	rBV	137593	295567	43.22%	4.885%
13	6.986	1839	1849	1870	rBV2	46943	95614	13.98%	1.580%
14	7.314	1938	1951	1969	rBV	223591	407527	59.59%	6.736%
15	7.625	2037	2048	2061	rBV2	25590	50434	7.37%	0.834%
16	8.088	2181	2192	2225	rBV	297364	663388	97.01%	10.965%
17	8.847	2417	2428	2457	rBV2	339027	662343	96.85%	10.948%
18	9.011	2470	2479	2490	rBV	28041	47072	6.88%	0.778%
19	9.140	2511	2519	2528	rBV9	5618	10565	1.54%	0.175%
20	9.548	2637	2646	2651	rBV9	4926	9256	1.35%	0.153%
21	9.928	2756	2764	2773	rBV4	10667	19610	2.87%	0.324%
22	10.211	2839	2852	2864	rBV	97201	158218	23.14%	2.615%
23	10.371	2887	2902	2913	rVB8	10653	22688	3.32%	0.375%
24	11.243	3162	3173	3191	rBV	311788	503179	73.58%	8.317%
25	11.522	3252	3260	3262	rBV6	8171	9629	1.41%	0.159%
26	11.616	3279	3289	3307	rBV	212653	354272	51.81%	5.856%




Sum of corrected areas: 6049955

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028755.D
Acq On : 28 Oct 2022 14:31
Operator : SY/MD
Sample : N5233-08DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

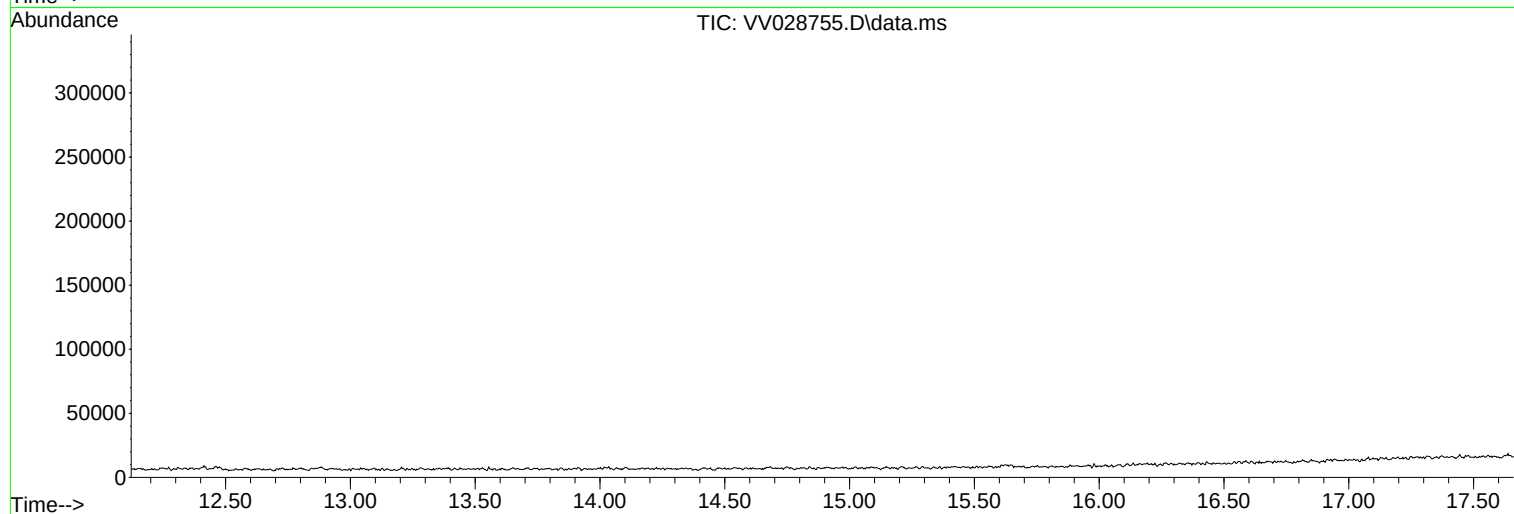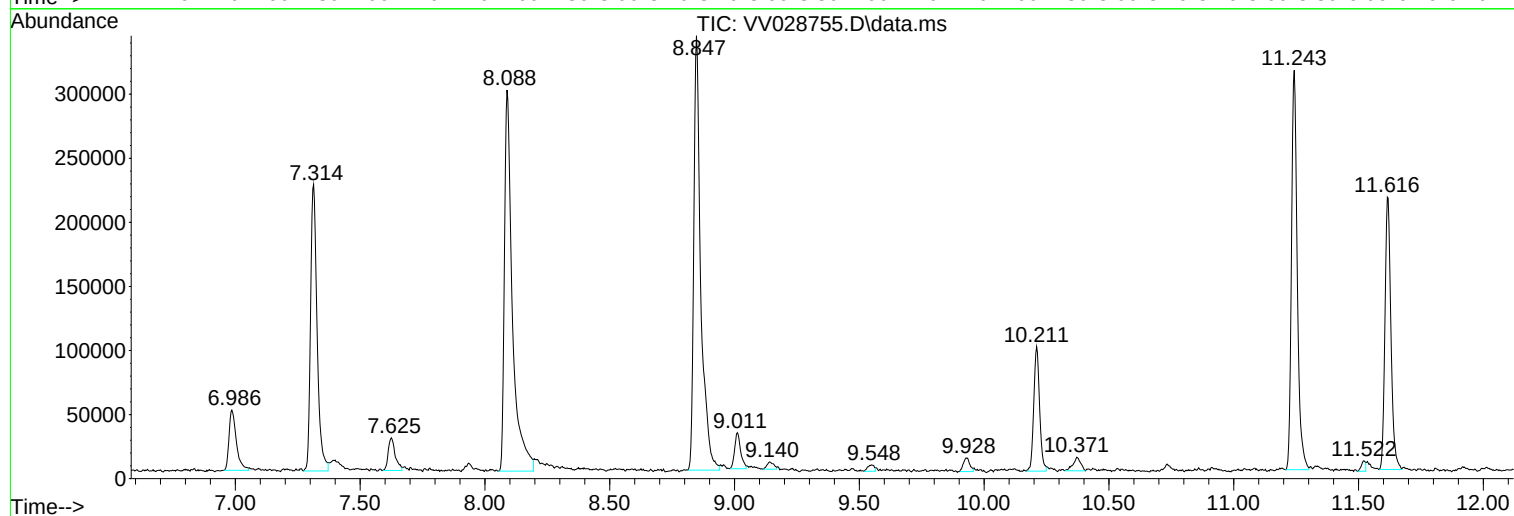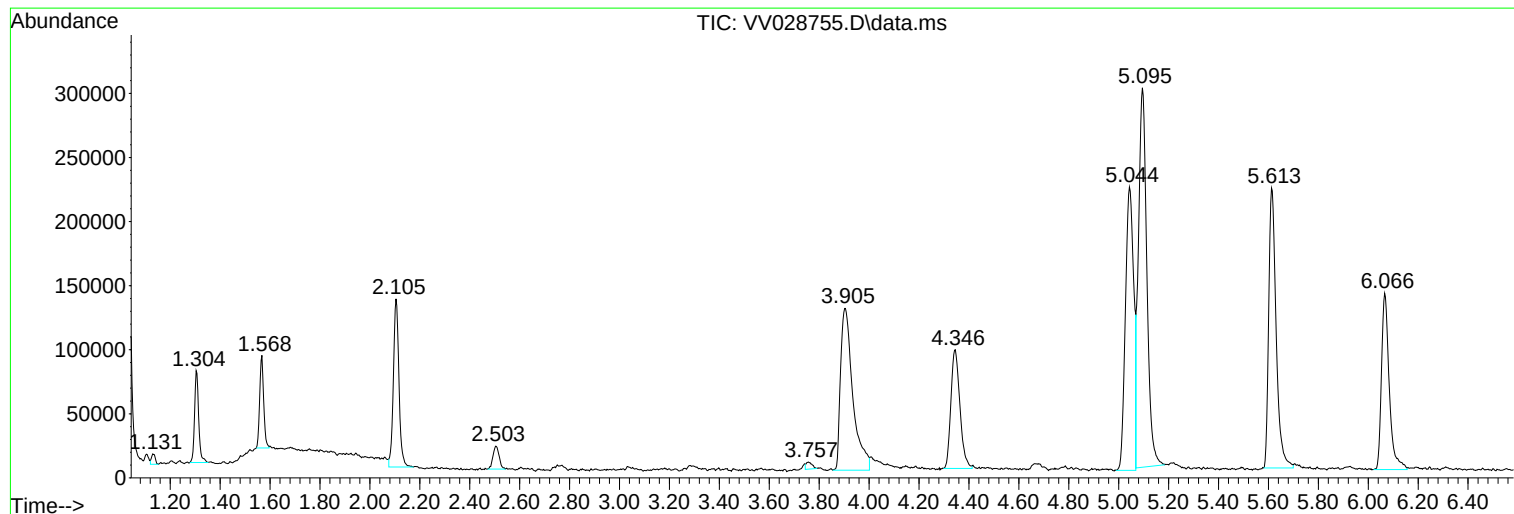

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028755.D
Acq On : 28 Oct 2022 14:31
Operator : SY/MD
Sample : N5233-08DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028755.D
Acq On : 28 Oct 2022 14:31
Operator : SY/MD
Sample : N5233-08DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA76DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc