

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
 Data File : VV028759.D
 Acq On : 28 Oct 2022 16:06
 Operator : SY/MD
 Sample : N5232-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	60720	65542	10.62%	1.290%
2	1.568	157	164	178	rVB	70086	84346	13.67%	1.661%
3	2.104	322	331	345	rVB	124730	183170	29.69%	3.606%
4	2.178	345	354	369	rVB2	9790	21592	3.50%	0.425%
5	3.892	876	887	923	rBV2	79497	273800	44.38%	5.390%
6	4.355	1013	1031	1058	rBV3	117391	409265	66.34%	8.057%
7	5.043	1227	1245	1271	rBV2	208733	543122	88.04%	10.693%
8	5.616	1411	1423	1451	rBV	213349	452308	73.32%	8.905%
9	6.066	1551	1563	1586	rBV	133111	278051	45.07%	5.474%
10	6.985	1838	1849	1866	rBV	47263	95097	15.42%	1.872%
11	7.313	1939	1951	1967	rBV	210281	383513	62.17%	7.550%
12	7.390	1970	1975	1988	rVB2	14831	28108	4.56%	0.553%
13	7.625	2039	2048	2066	rBV3	24779	49147	7.97%	0.968%
14	8.088	2183	2192	2216	rBV	295291	616908	100.00%	12.145%
15	8.252	2236	2243	2253	rVB	6422	11795	1.91%	0.232%
16	8.847	2416	2428	2448	rBV	322638	547559	88.76%	10.780%
17	9.143	2511	2520	2532	rBV3	7266	12197	1.98%	0.240%
18	9.545	2636	2645	2648	rBV9	4667	6271	1.02%	0.123%
19	10.210	2840	2852	2865	rBV	93030	152875	24.78%	3.010%
20	10.377	2895	2904	2911	rBV4	10100	15741	2.55%	0.310%
21	11.156	3137	3146	3153	rBV4	5089	8876	1.44%	0.175%
22	11.242	3163	3173	3193	rBV	306472	491132	79.61%	9.669%
23	11.619	3279	3290	3307	rBV	205276	339046	54.96%	6.675%
24	12.342	3510	3515	3524	rBV	5836	9902	1.61%	0.195%




Sum of corrected areas: 5079363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028759.D
Acq On : 28 Oct 2022 16:06
Operator : SY/MD
Sample : N5232-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

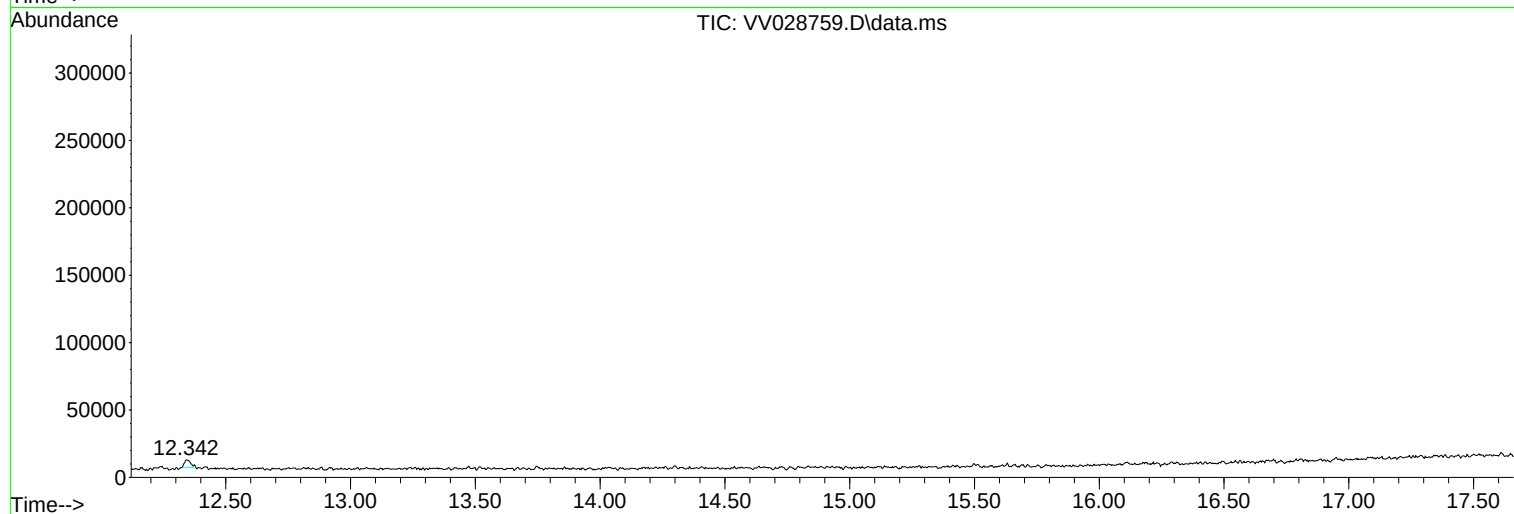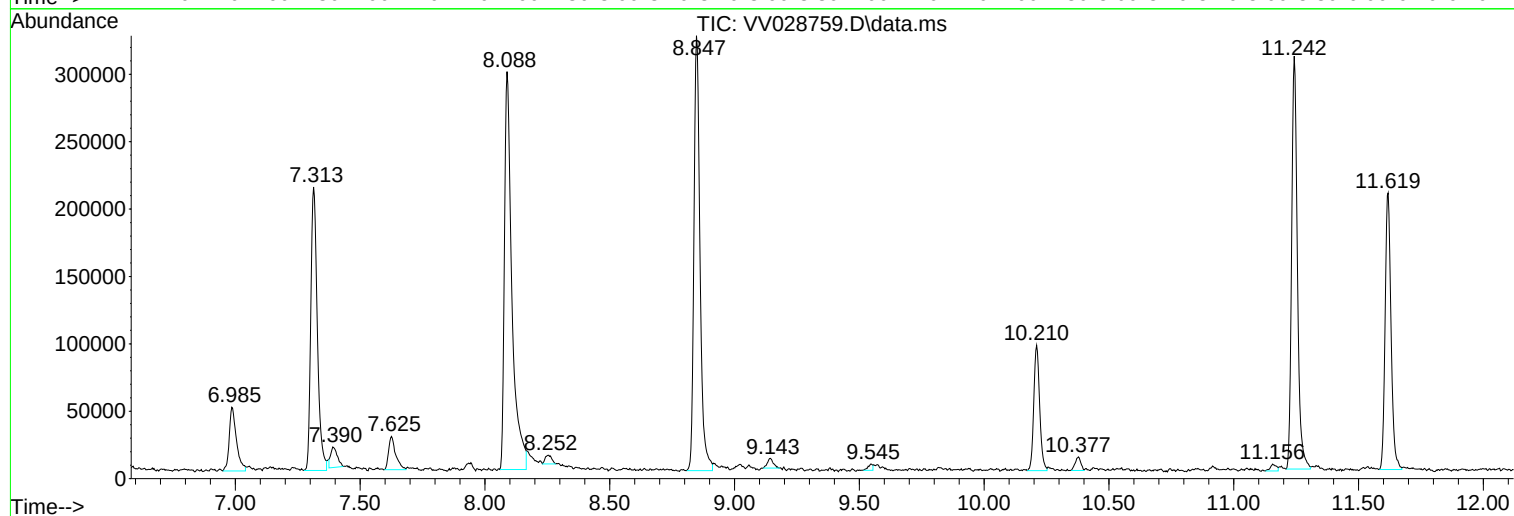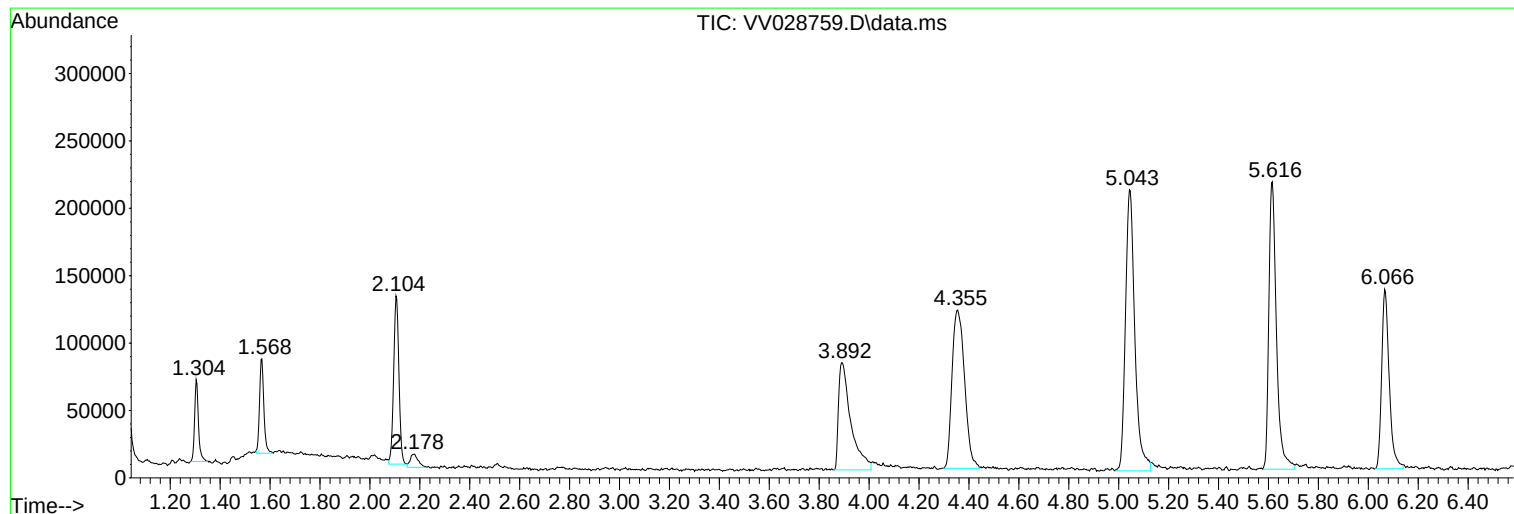

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028759.D
Acq On : 28 Oct 2022 16:06
Operator : SY/MD
Sample : N5232-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102822\
Data File : VV028759.D
Acq On : 28 Oct 2022 16:06
Operator : SY/MD
Sample : N5232-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc